

SUPERVISOR TEST




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 06/17/2017

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17120

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:07
INTERNAL STANDARD	VERIFIED	03:07
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	03:07
BLANK TEST	0.00	03:08
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	03:08
BLANK TEST	0.00	03:09
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	03:09
BLANK TEST	0.00	03:10

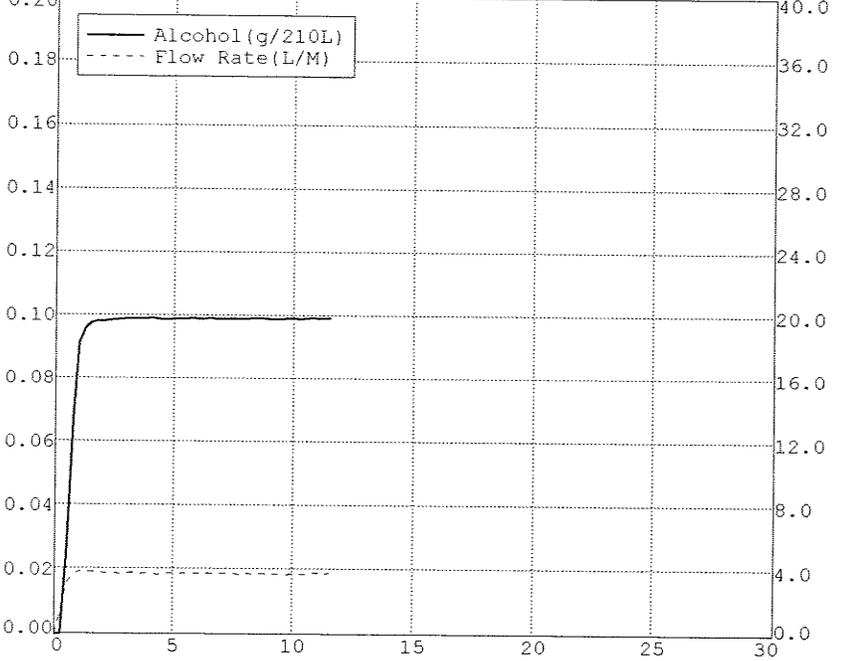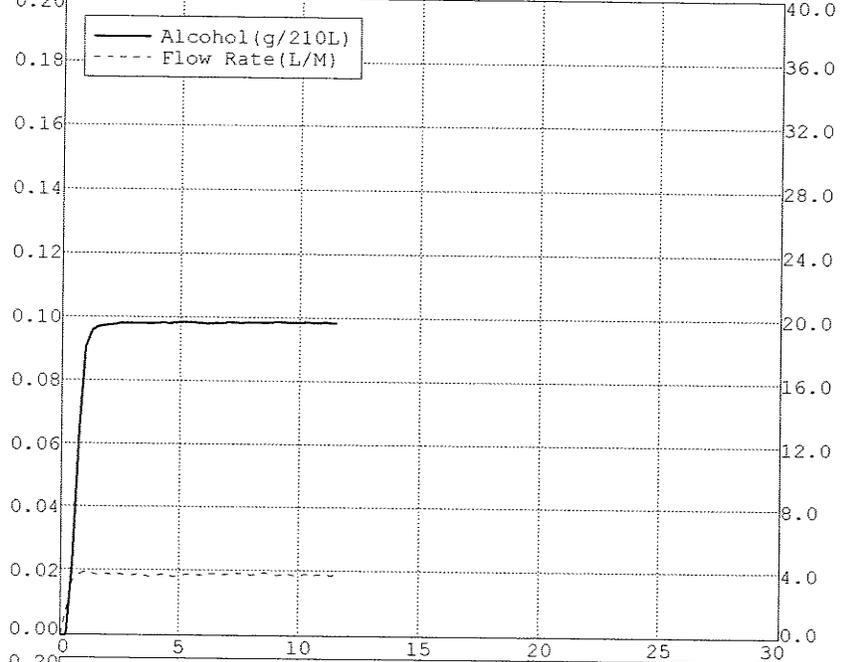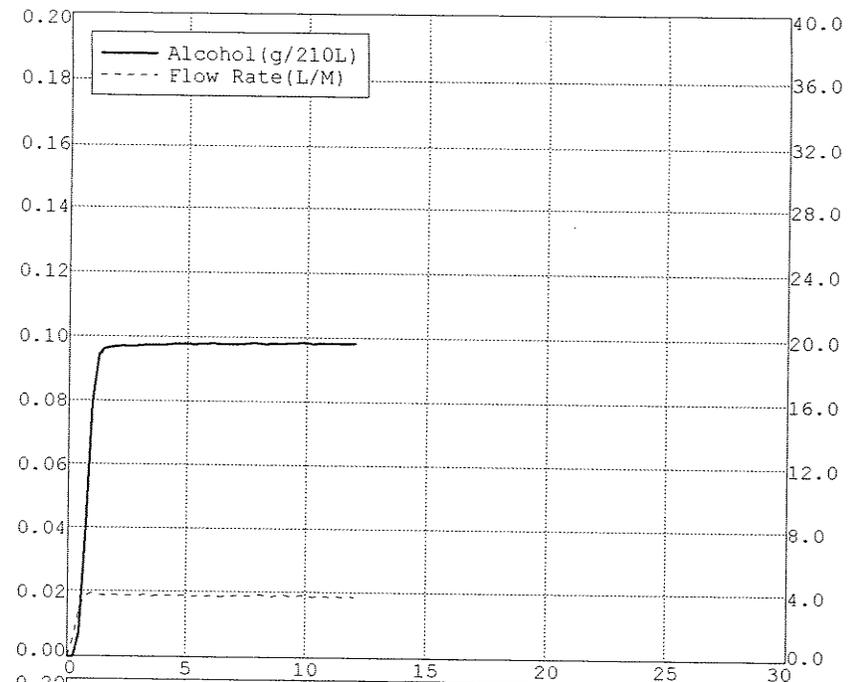

*Charles B. Geisler #241*