

SUPERVISOR TEST




WARREN COUNTY  
SHERRIF'S OFFICE  
DATAMASTER dmt: 144506

Date: 06/22/2017

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17120

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:24
INTERNAL STANDARD	VERIFIED	23:24
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	23:24
BLANK TEST	0.00	23:25
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	23:26
BLANK TEST	0.00	23:26
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	23:27
BLANK TEST	0.00	23:28

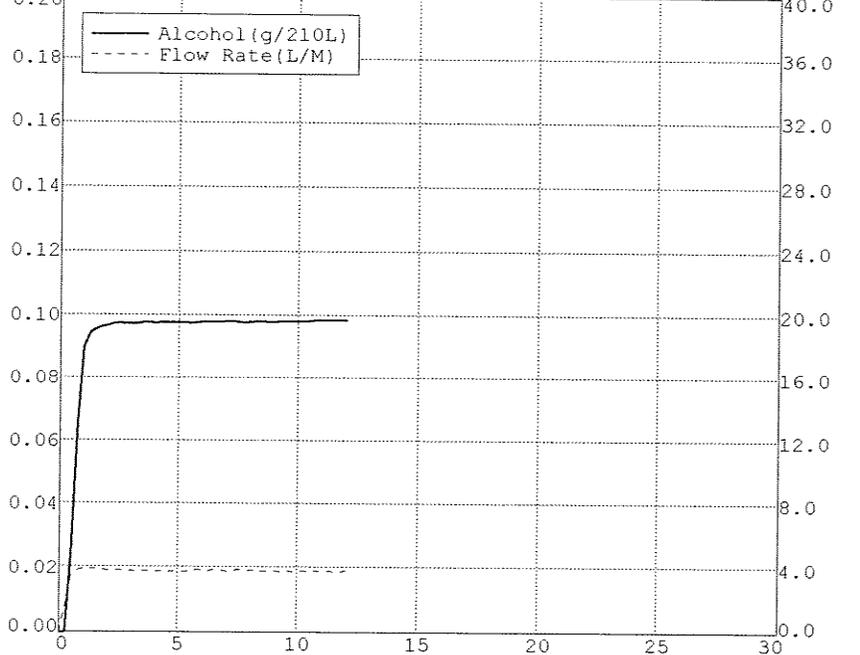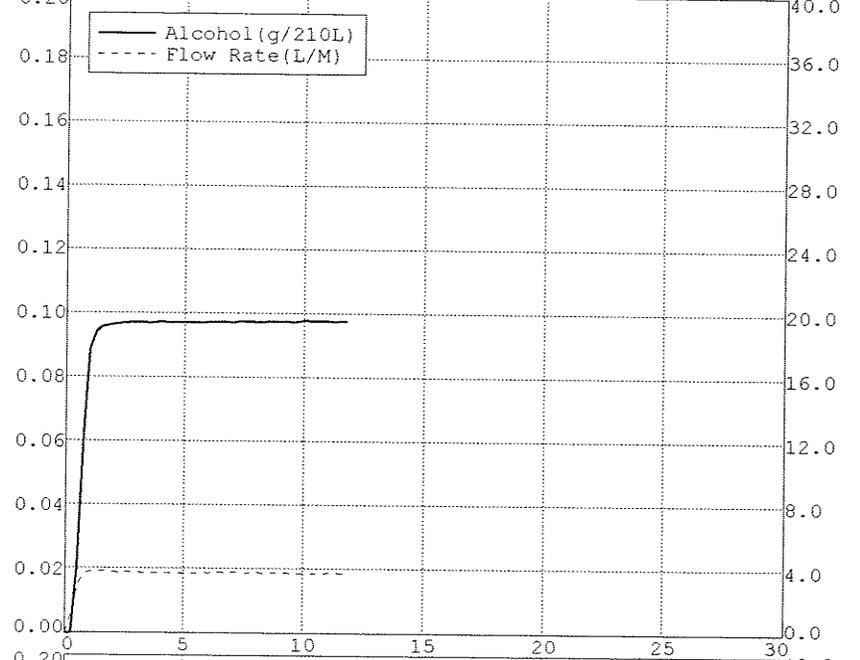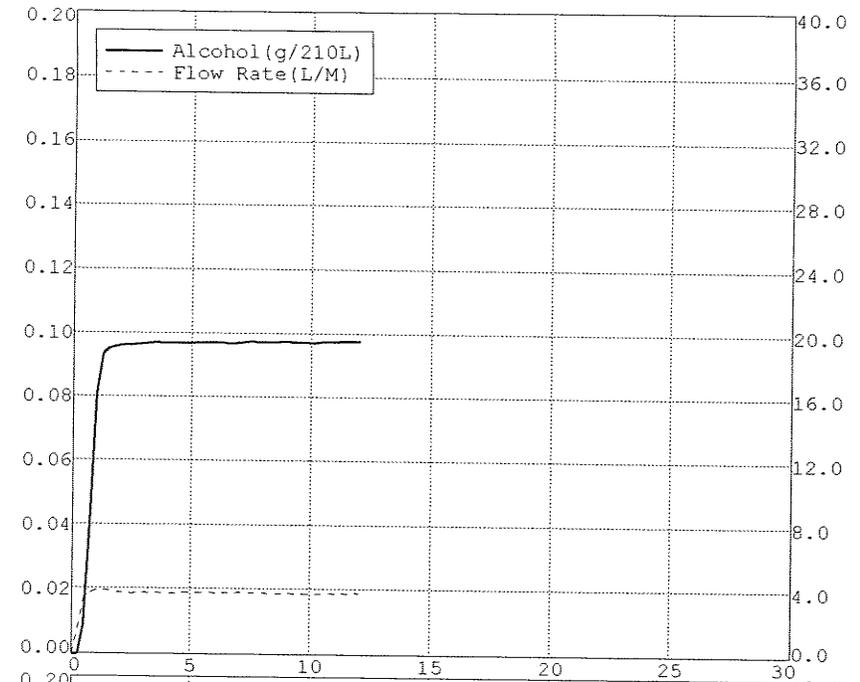

*Sp. Ch. B. [Signature]* #248