

SOLUTION CHANGE




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 07/01/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17120

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:48
INTERNAL STANDARD	VERIFIED	22:48
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	22:49
BLANK TEST	0.00	22:49
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	22:50
BLANK TEST	0.00	22:51
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.10	22:51
BLANK TEST	0.00	22:52

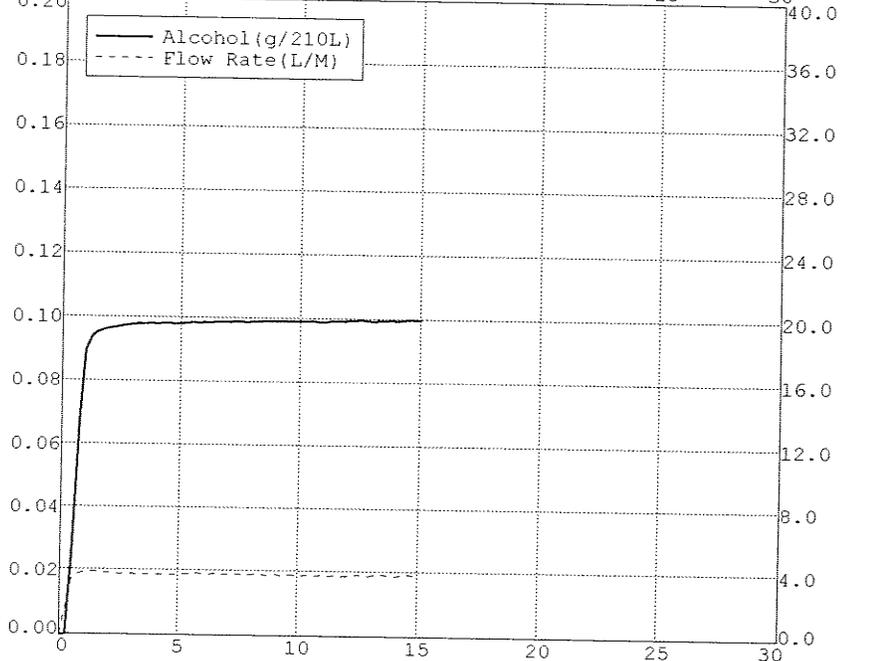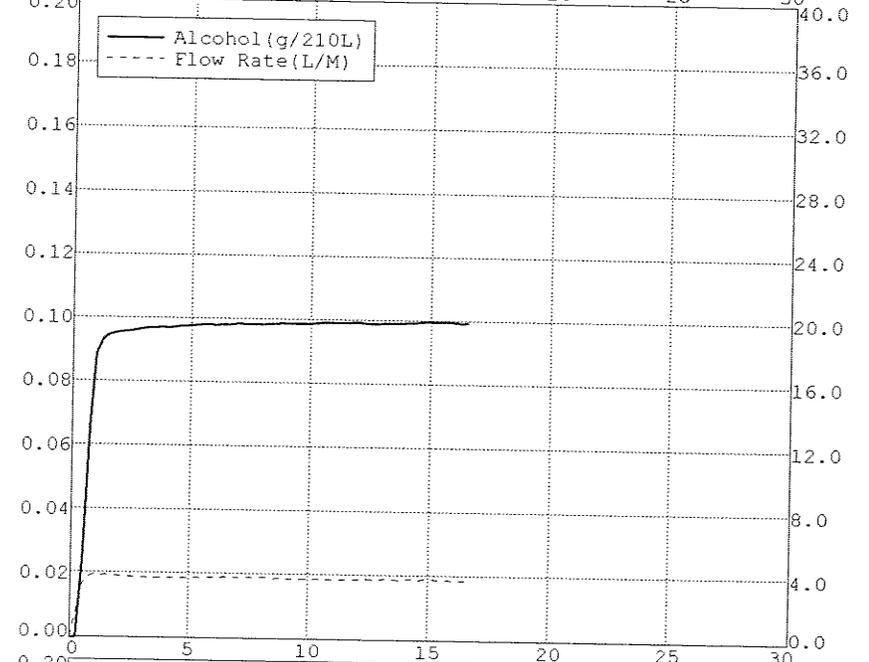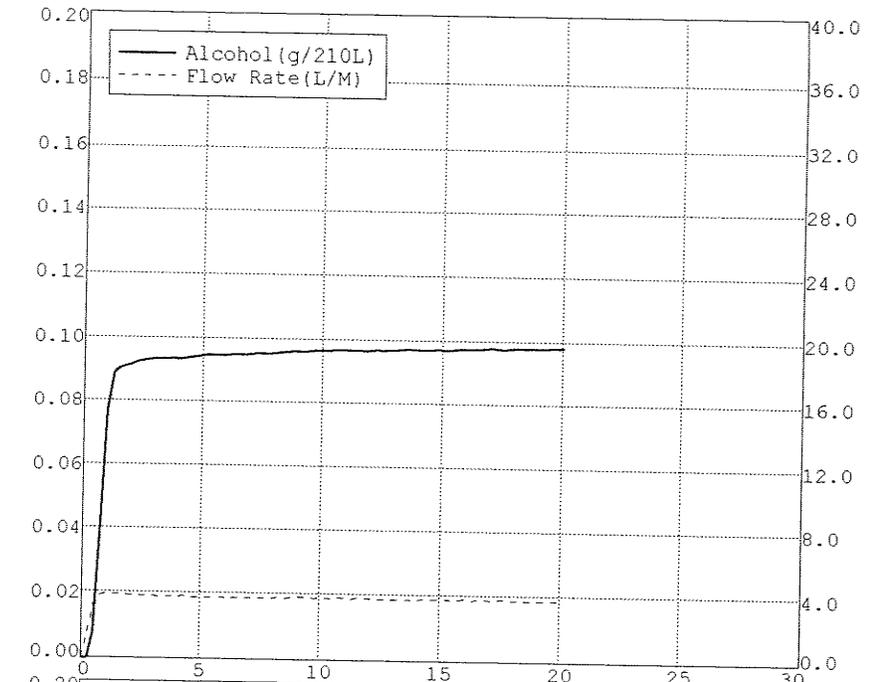

Charles B. Geisler #241