

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 07/17/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17120

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:25
INTERNAL STANDARD	VERIFIED	00:25
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:25
BLANK TEST	0.00	00:26
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	00:27
BLANK TEST	0.00	00:27
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:28
BLANK TEST	0.00	00:29

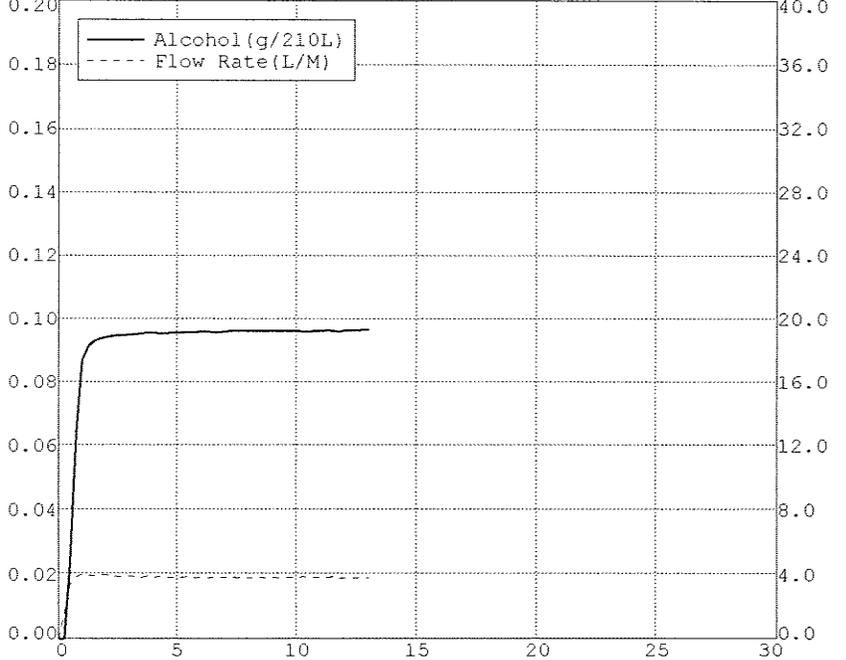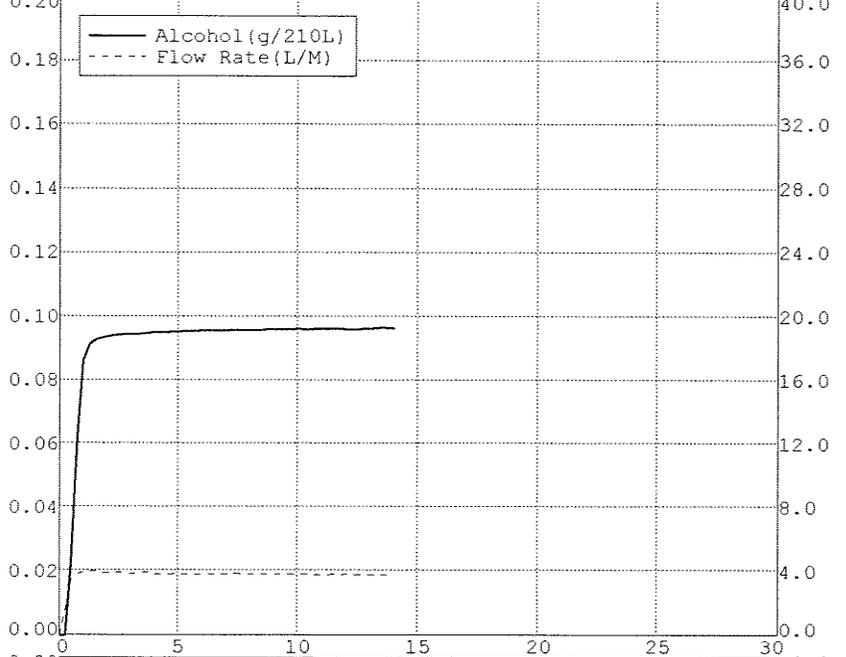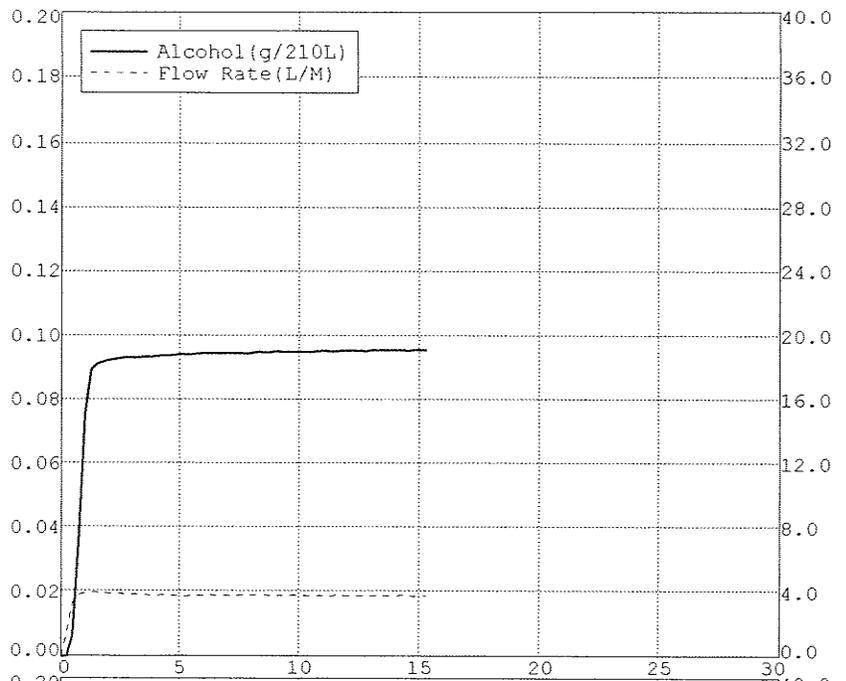

Sgt. Charles B. Geisler #241