

SUPERVISOR TEST




WARREN COUNTY
SHERRIF'S OFFICE
DATAMASTER dmt: 144506

Date: 07/25/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17120

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:57
INTERNAL STANDARD	VERIFIED	01:57
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	01:57
BLANK TEST	0.00	01:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	01:58
BLANK TEST	0.00	01:59
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	01:59
BLANK TEST	0.00	02:00

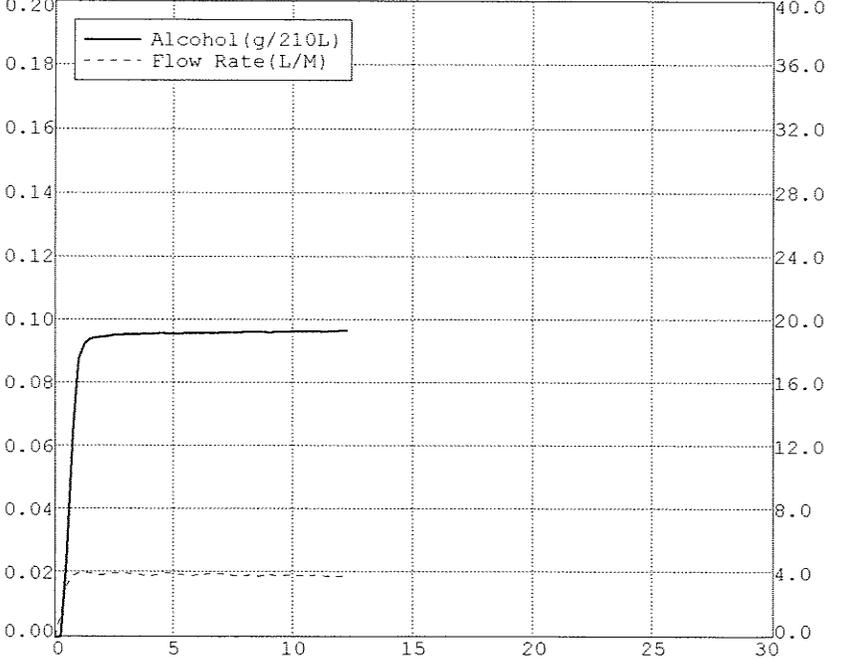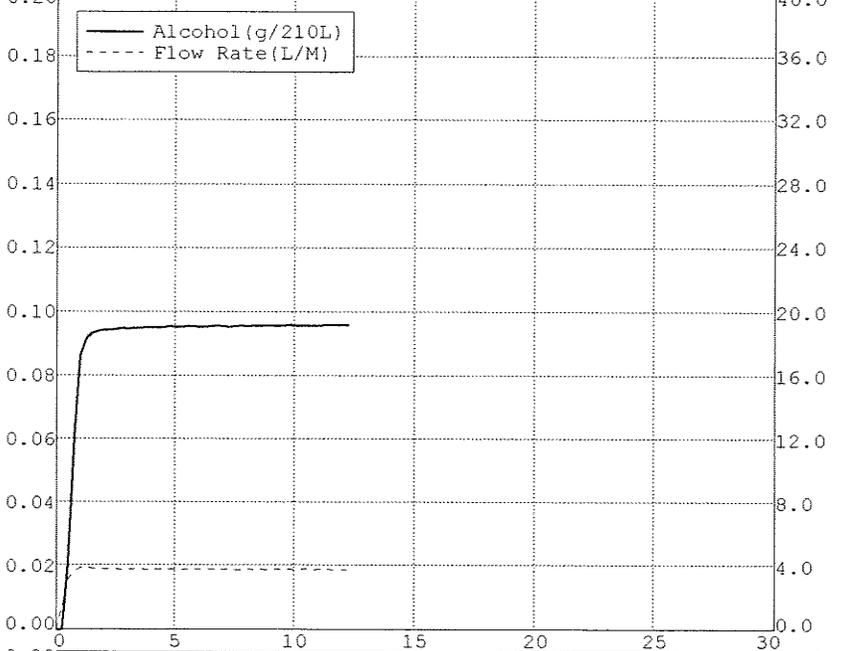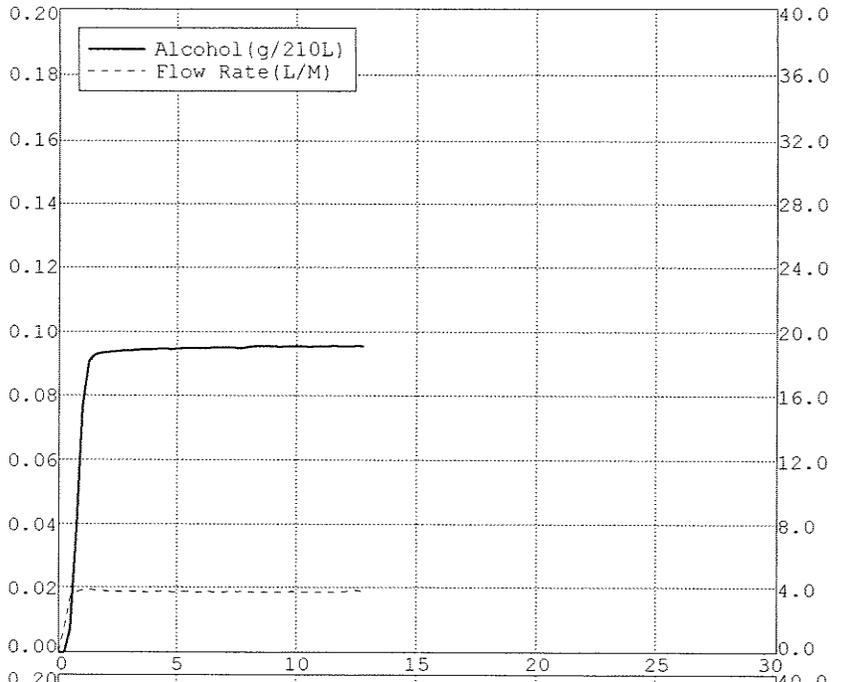

Sup. Charles B. Geisler #248