

SUPERVISOR TEST




WARREN COUNTY  
SHERRIF'S OFFICE  
DATAMASTER dmt: 144506

Date: 07/30/2017

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17120

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:03
INTERNAL STANDARD	VERIFIED	02:03
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	02:03
BLANK TEST	0.00	02:04
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	02:05
BLANK TEST	0.00	02:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:06
BLANK TEST	0.00	02:07

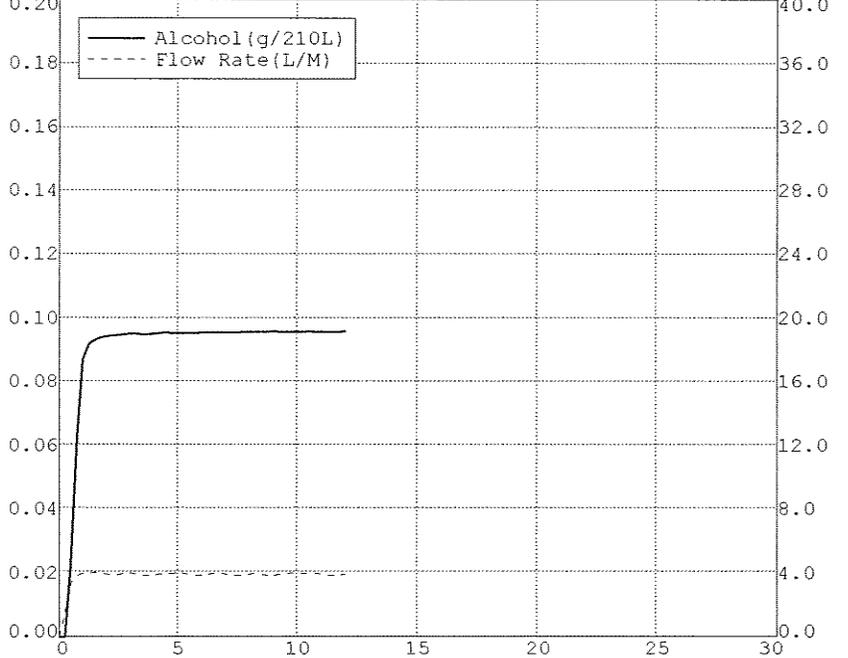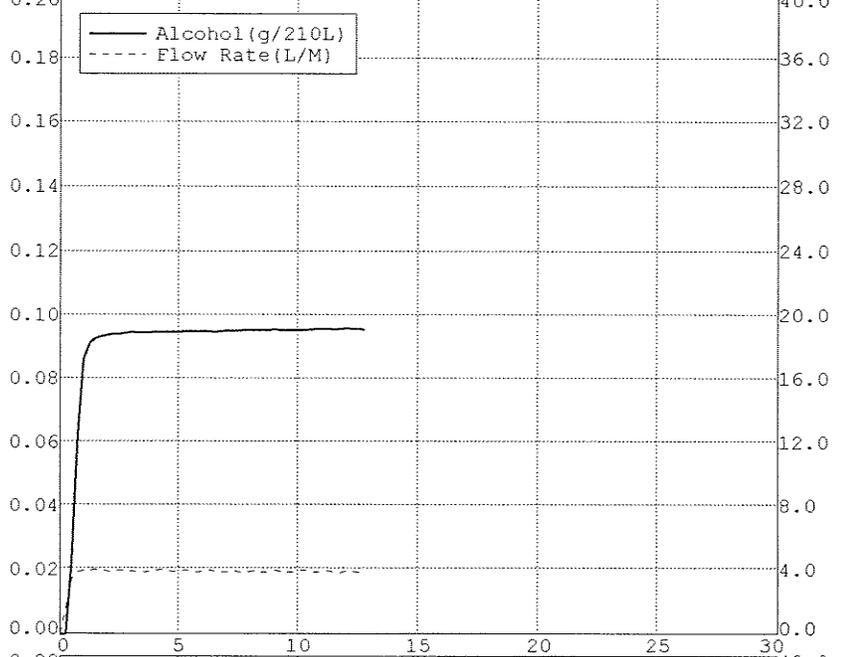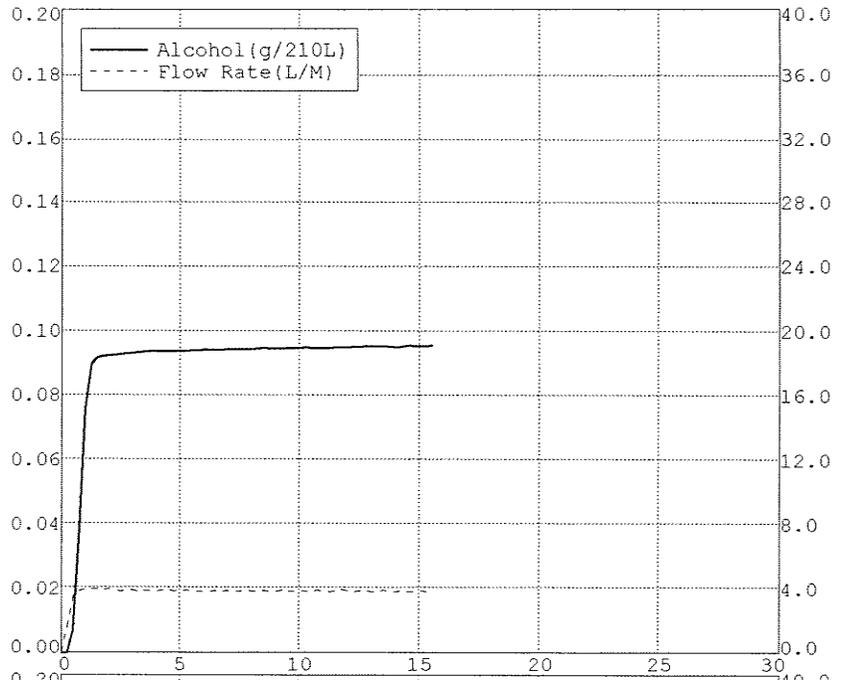

*Charles B. Geisler #244*