

SUPERVISOR TEST




WARREN COUNTY  
SHERRIF'S OFFICE  
DATAMASTER dmt: 144506

Date: 08/11/2017

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17150

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:04
INTERNAL STANDARD	VERIFIED	23:04
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	23:04
BLANK TEST	0.00	23:05
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	23:05
BLANK TEST	0.00	23:06
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	23:07
BLANK TEST	0.00	23:08

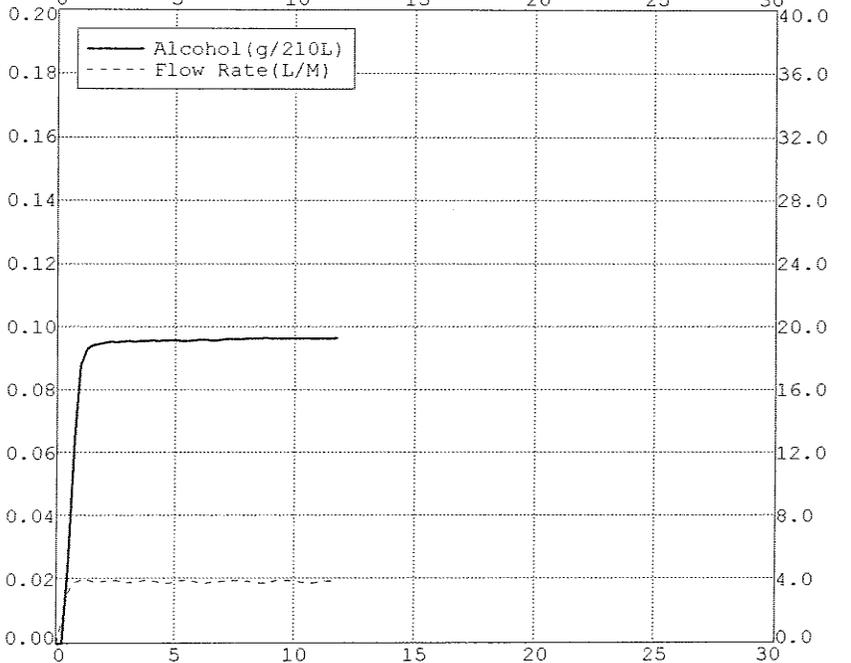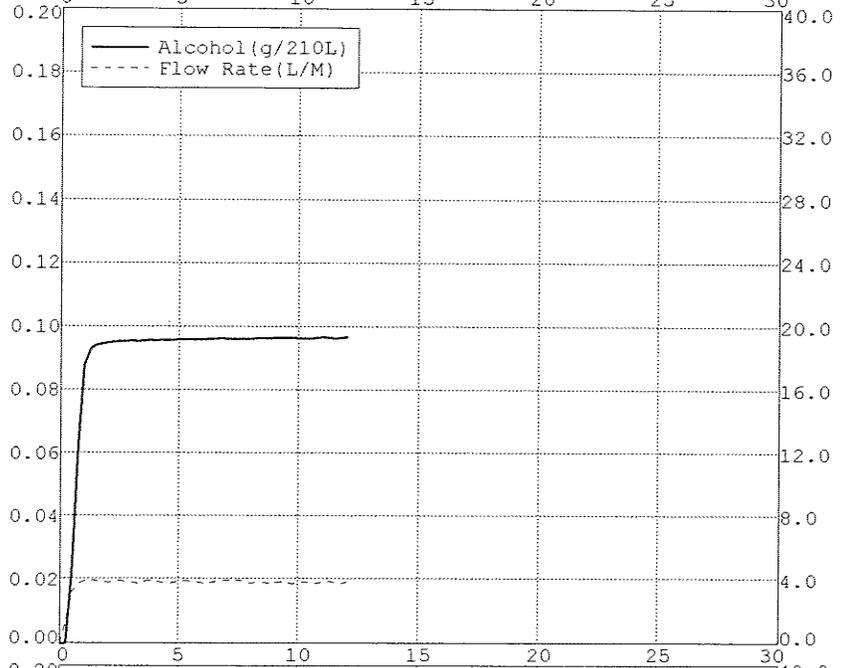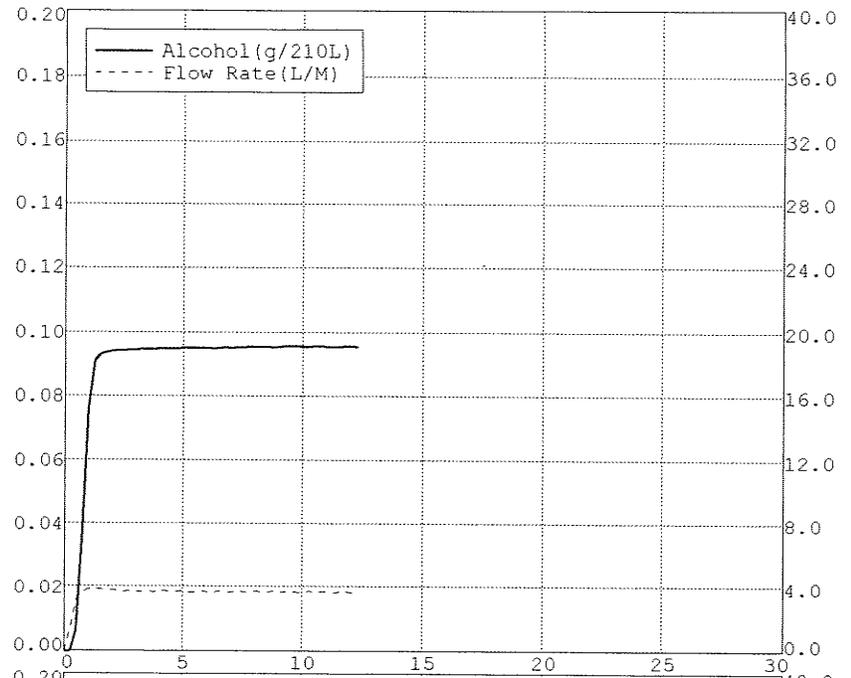

*Charles B. Geisler #241*