

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 08/21/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17150

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:50
INTERNAL STANDARD	VERIFIED	22:51
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	22:51
BLANK TEST	0.00	22:52
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	22:52
BLANK TEST	0.00	22:53
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	22:53
BLANK TEST	0.00	22:54

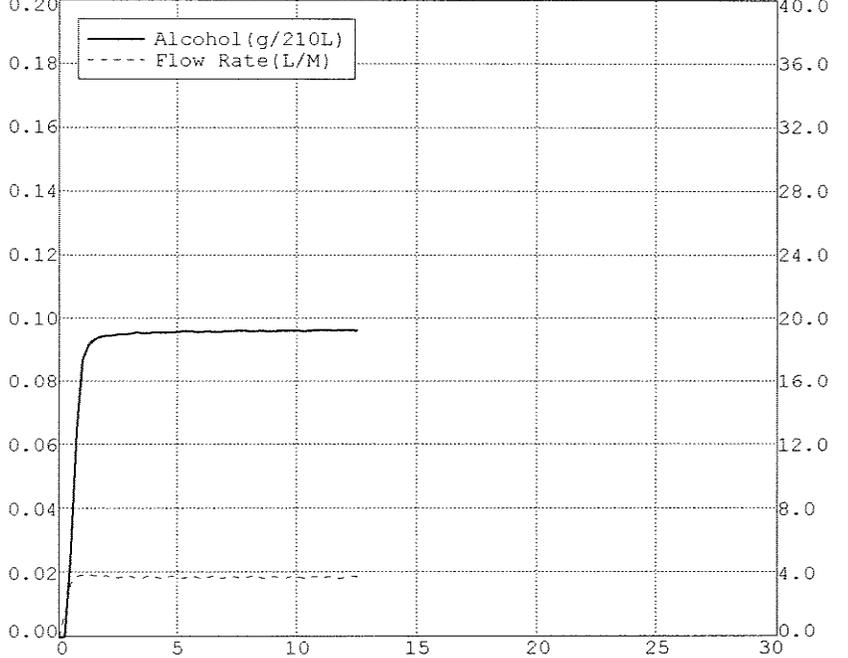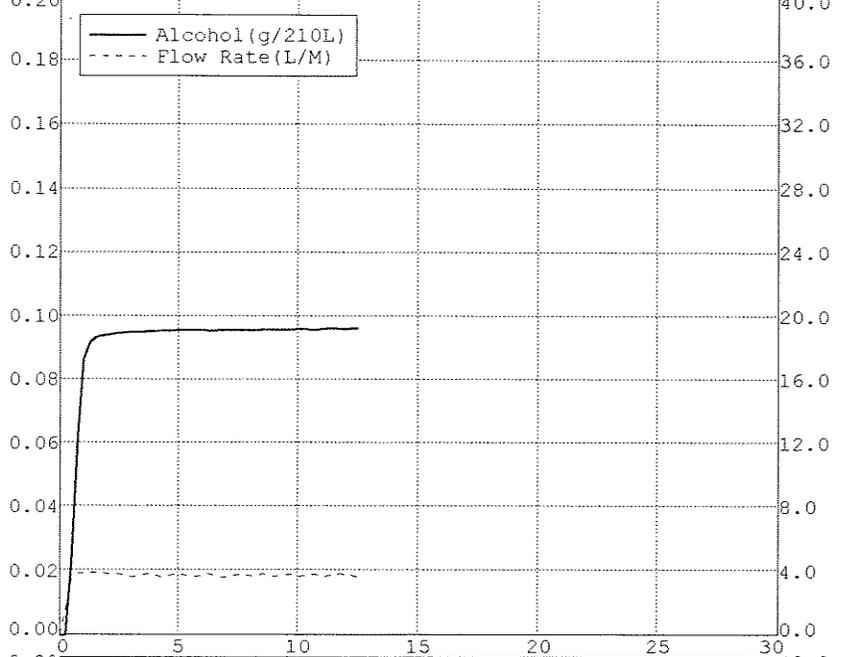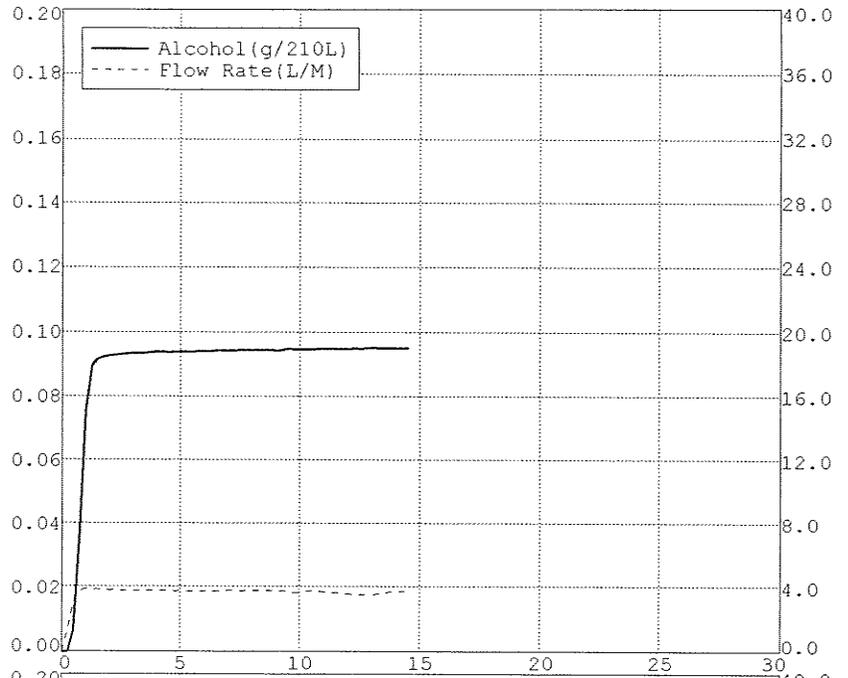

Sp. Ch. to Olf #2415