

SUPERVISOR TEST




WARREN COUNTY
SHERRIF'S OFFICE
DATAMASTER dmt: 144506

Date: 08/27/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17150

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:36
INTERNAL STANDARD	VERIFIED	21:36
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	21:36
BLANK TEST	0.00	21:37
REFERENCE STANDARD TEMP	34.04c	
REFERENCE STANDARD	0.09	21:38
BLANK TEST	0.00	21:38
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	21:39
BLANK TEST	0.00	21:40

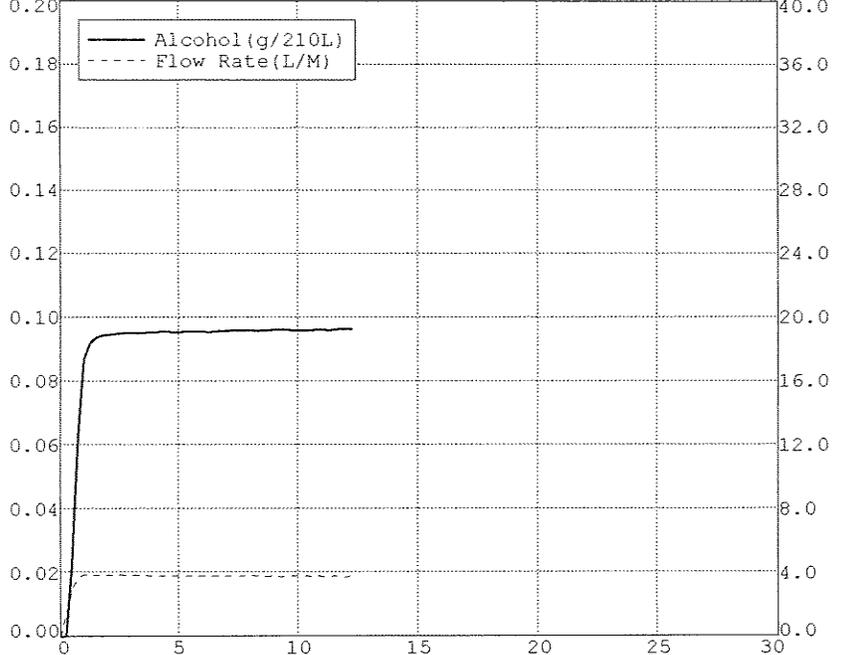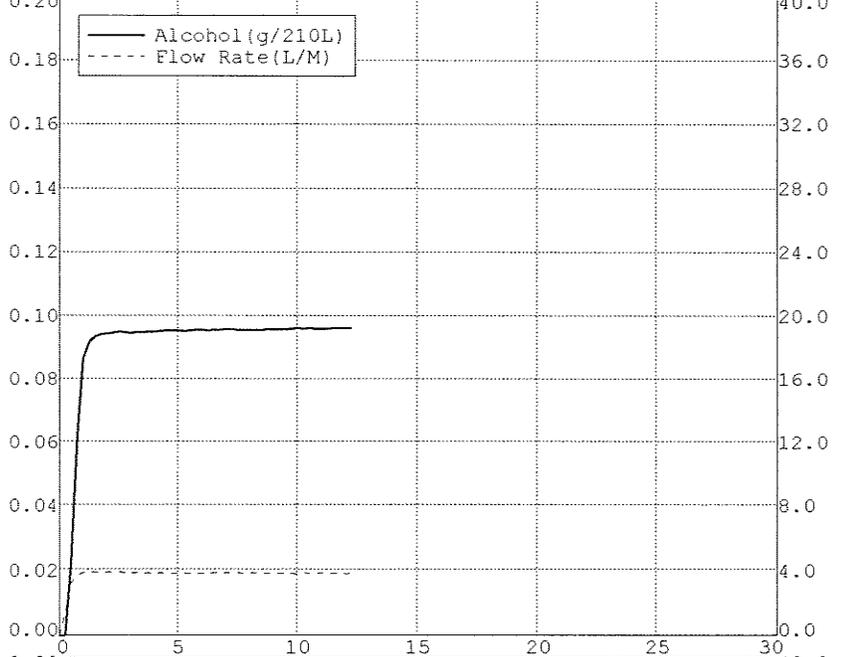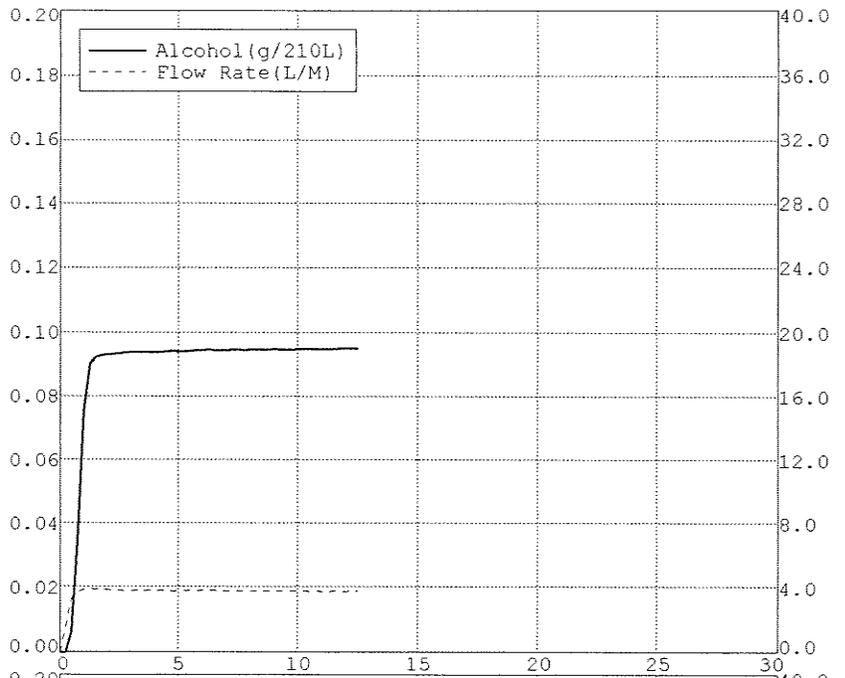

Charles B. Geisler