

SUPERVISOR TEST




WARREN COUNTY  
SHERRIF'S OFFICE  
DATAMASTER dmt: 144506

Date: 09/08/2017

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17150

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:59
INTERNAL STANDARD	VERIFIED	21:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:59
BLANK TEST	0.00	22:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	22:01
BLANK TEST	0.00	22:02
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	22:02
BLANK TEST	0.00	22:03

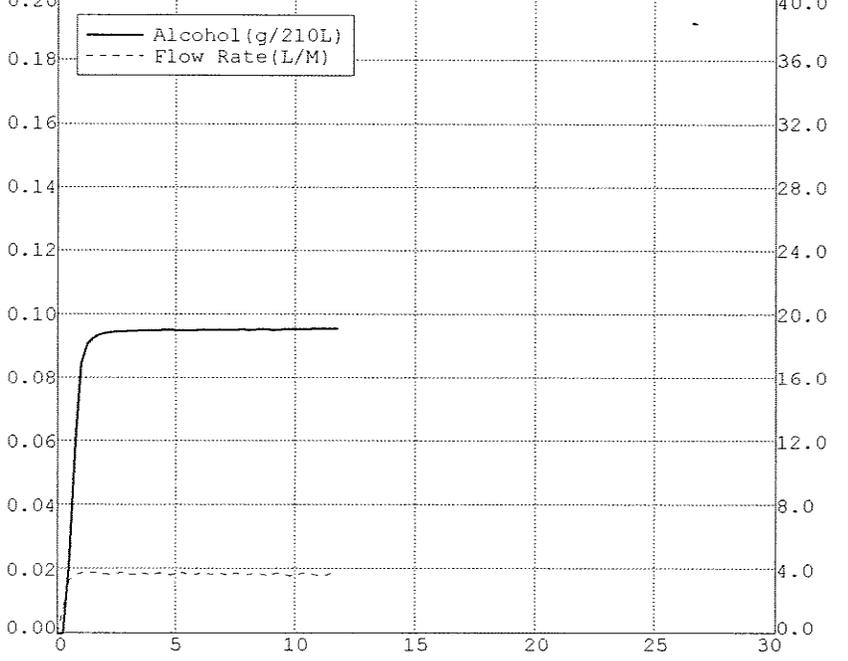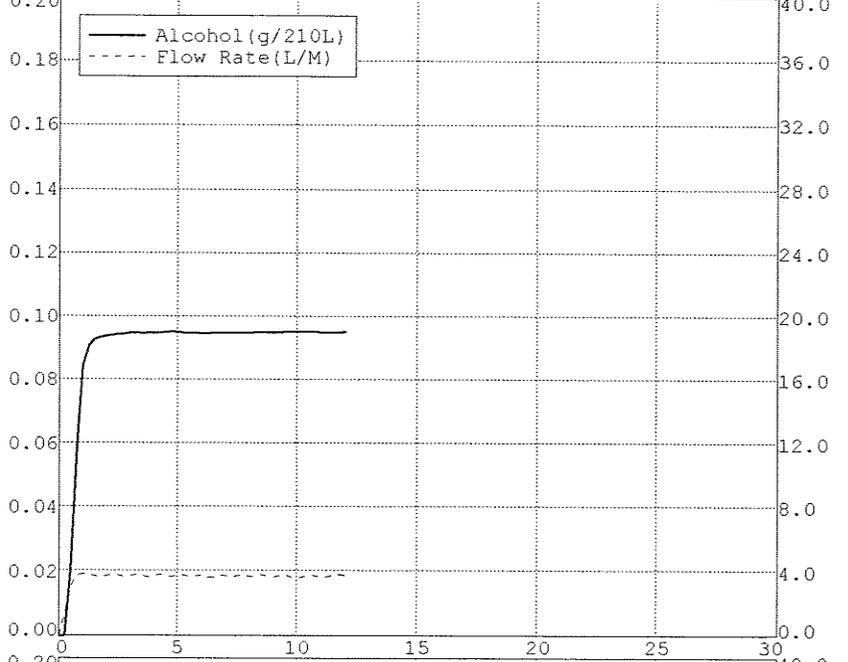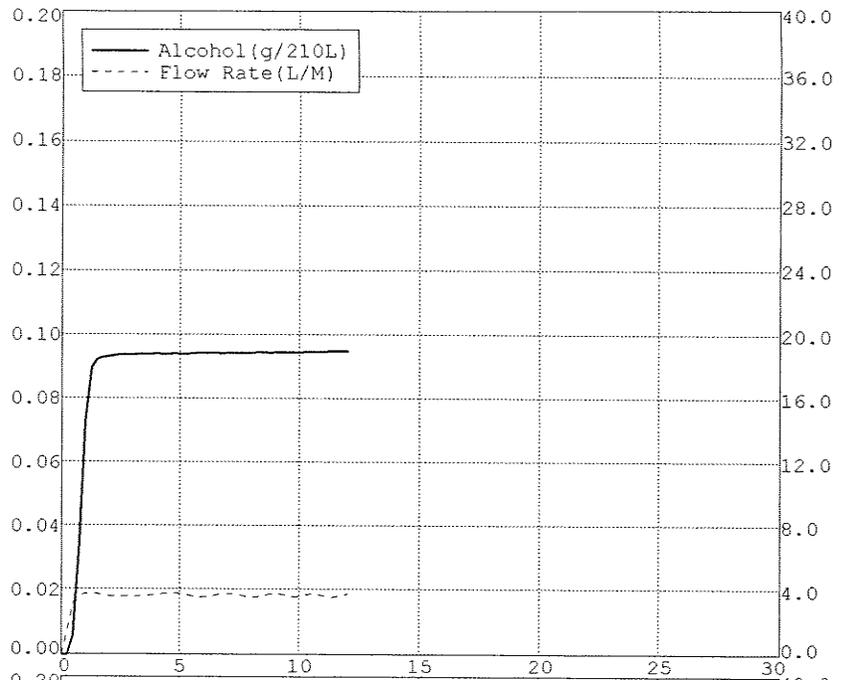

*Charles B. Geisler* #245