

SUPERVISOR TEST




WARREN COUNTY
 SHERRIF'S OFFICE
 DATAMASTER dmt: 144506

Date: 09/19/2017

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 17150

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:28
INTERNAL STANDARD	VERIFIED	02:28
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	02:29
BLANK TEST	0.00	02:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:30
BLANK TEST	0.00	02:31
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	02:31
BLANK TEST	0.00	02:32

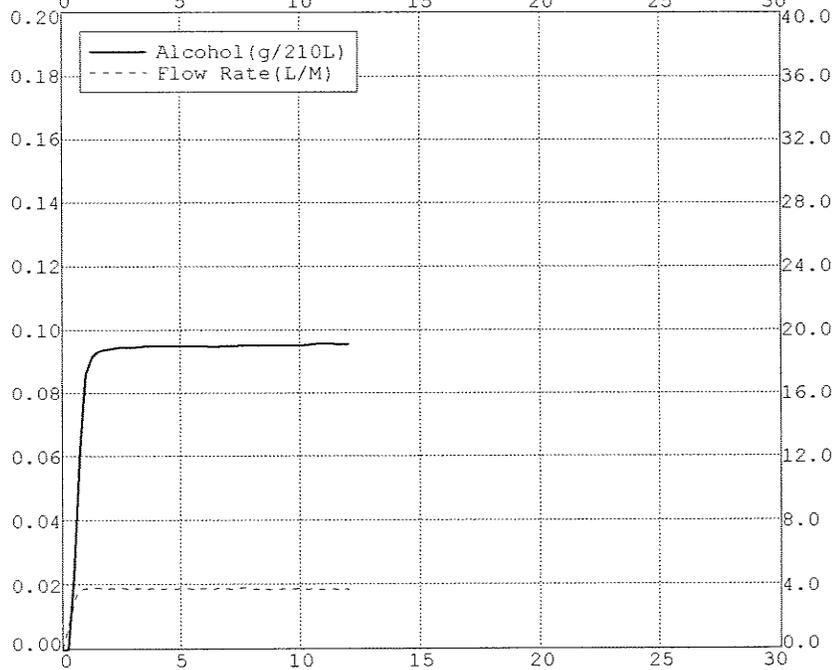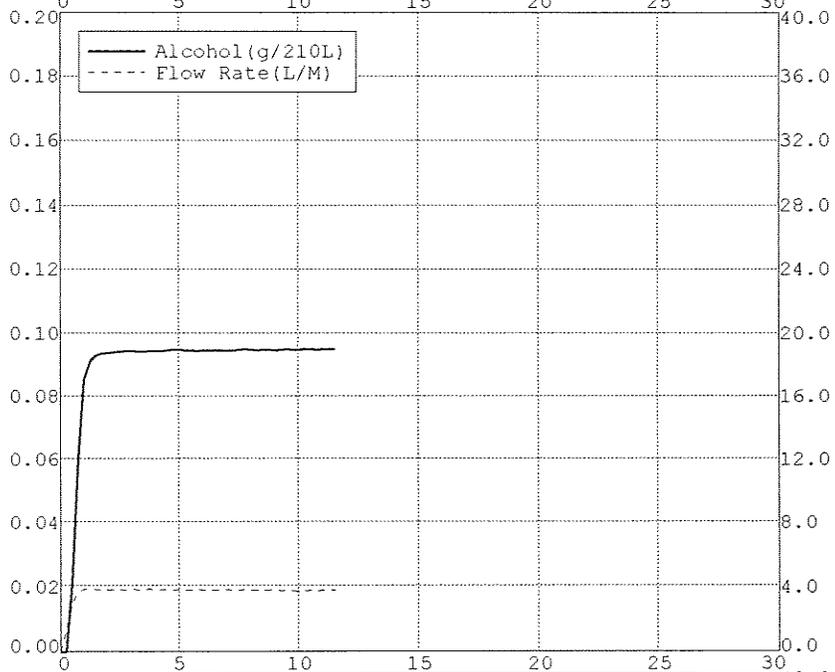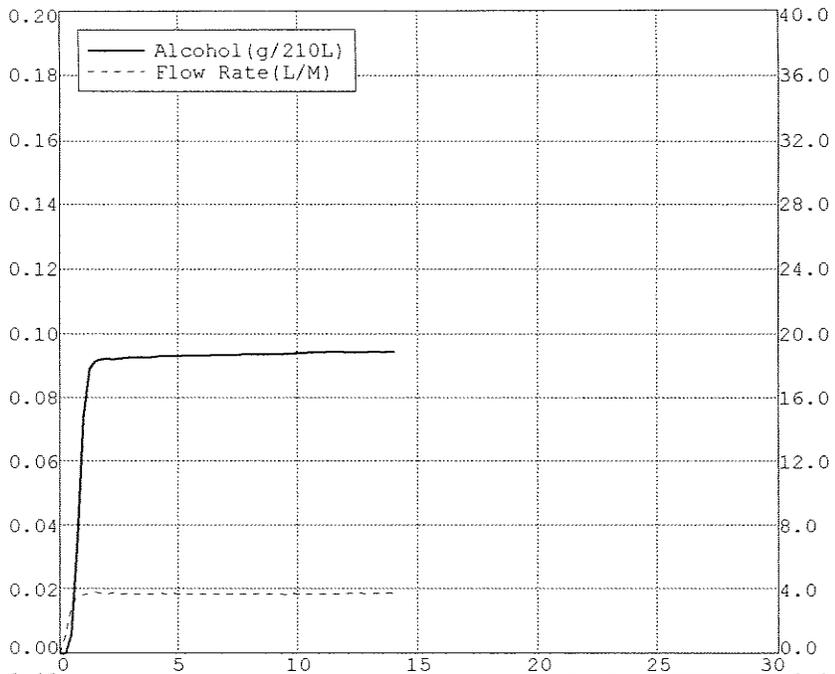

Sp. Ch. B. Q/S #241