

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 09/25/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17150

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:32
INTERNAL STANDARD	VERIFIED	00:33
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:33
BLANK TEST	0.00	00:34
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	00:34
BLANK TEST	0.00	00:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:35
BLANK TEST	0.00	00:36

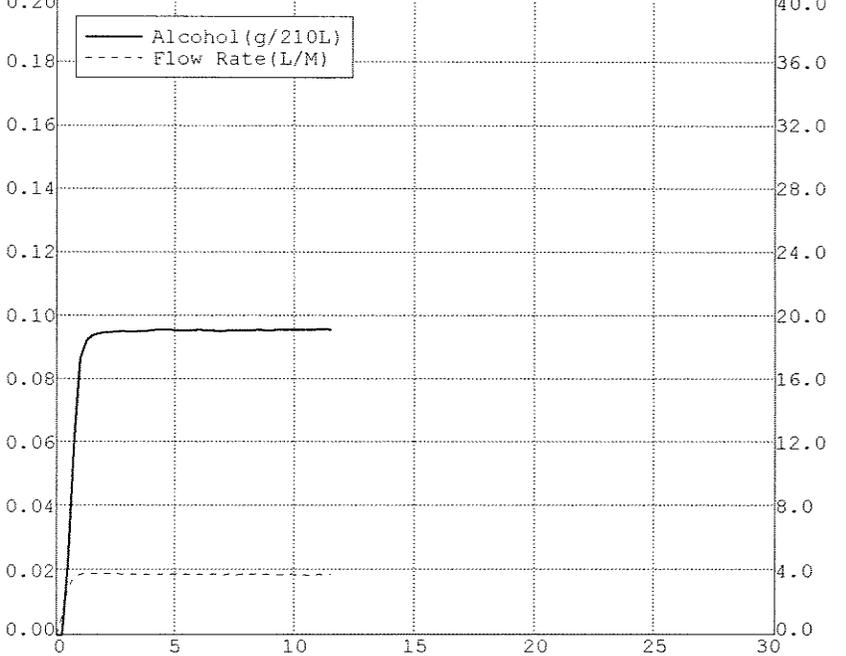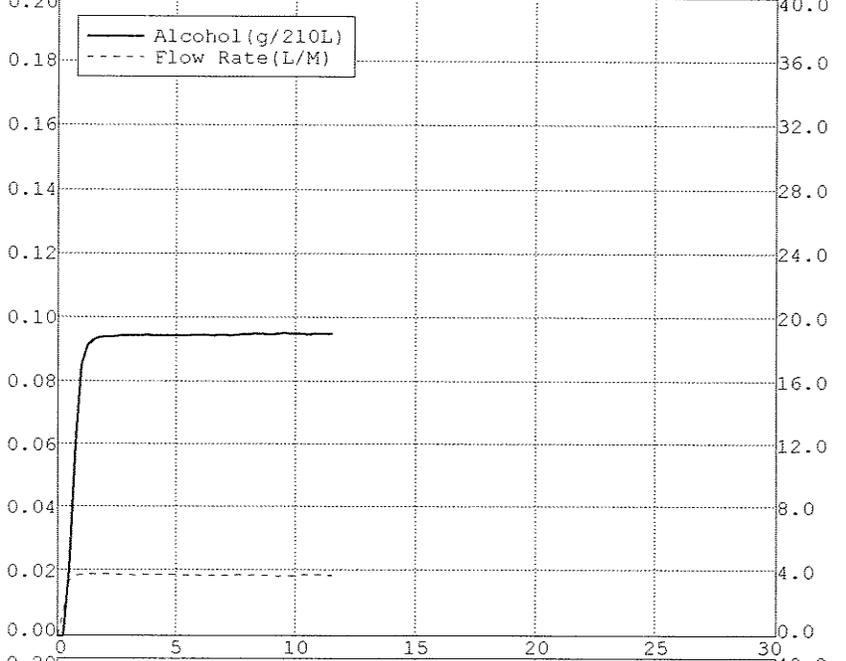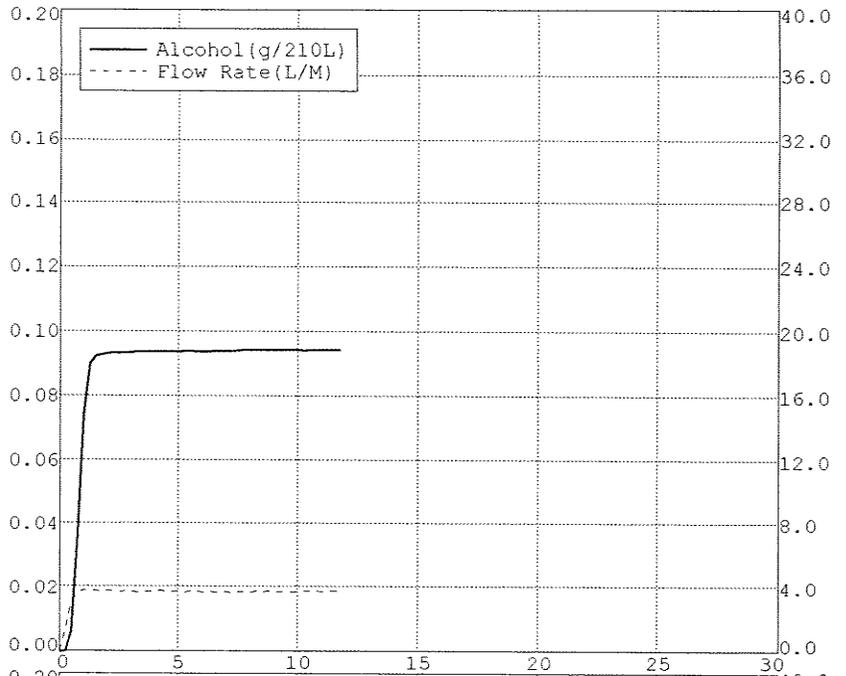

Charles B. Geisler #24