

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 10/16/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17720

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:43
INTERNAL STANDARD	VERIFIED	23:43
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	23:43
BLANK TEST	0.00	23:44
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	23:45
BLANK TEST	0.00	23:46
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	23:46
BLANK TEST	0.00	23:47

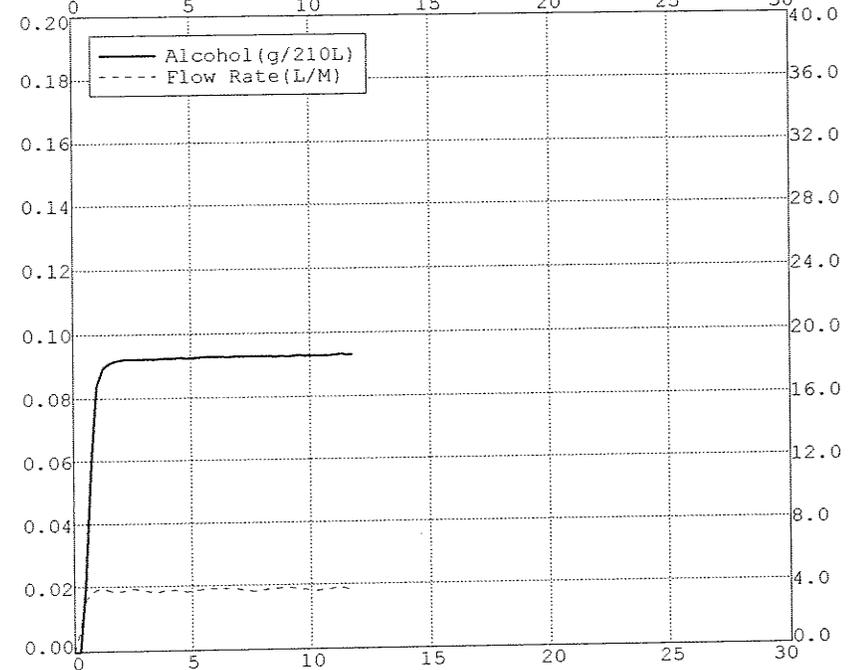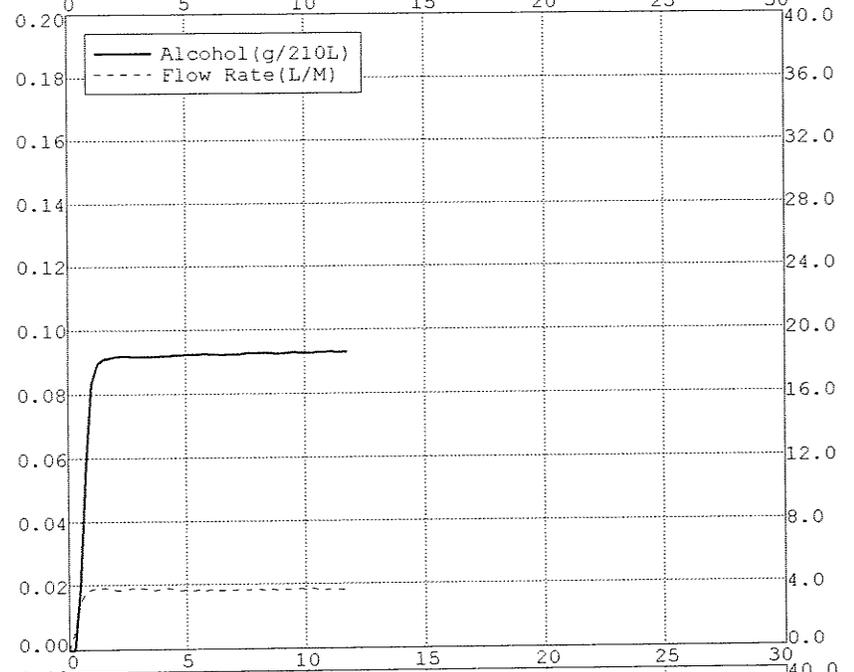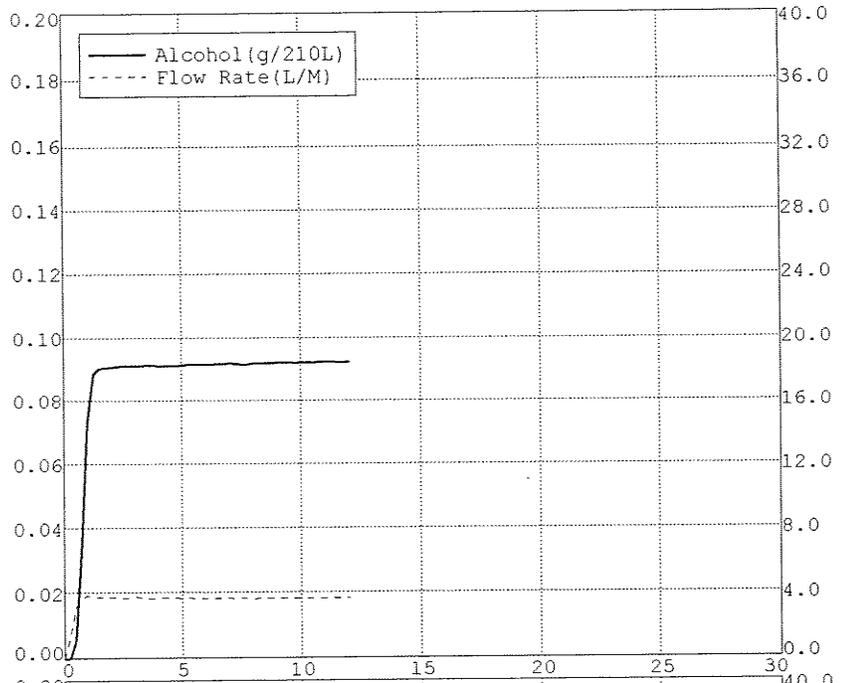

Charles B Geisler #210