

SUPERVISOR TEST




WARREN COUNTY
 SHERRIF'S OFFICE
 DATAMASTER dmt: 144506

Date: 10/22/2017

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 17220

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:08
INTERNAL STANDARD	VERIFIED	21:08
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	21:09
BLANK TEST	0.00	21:09
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	21:10
BLANK TEST	0.00	21:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:11
BLANK TEST	0.00	21:12

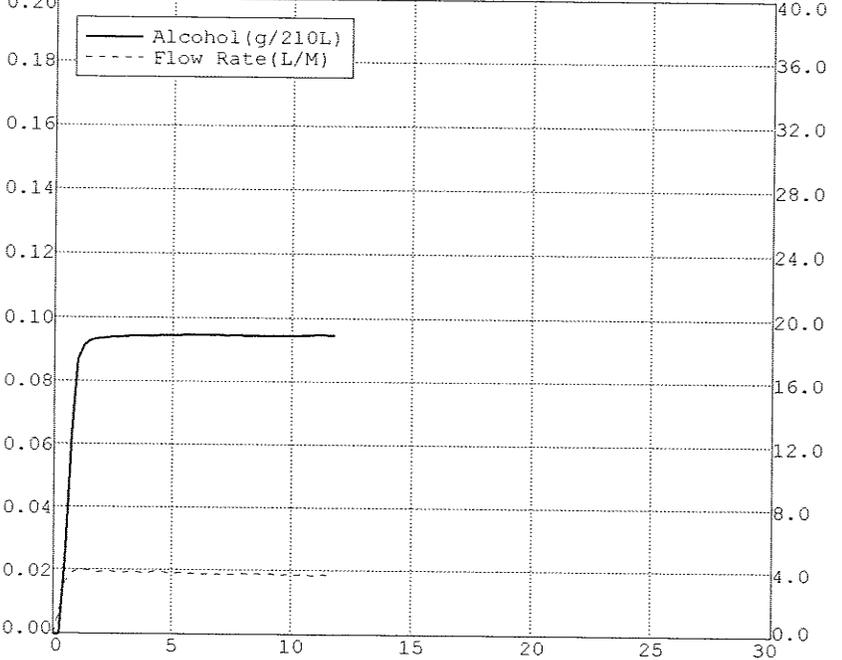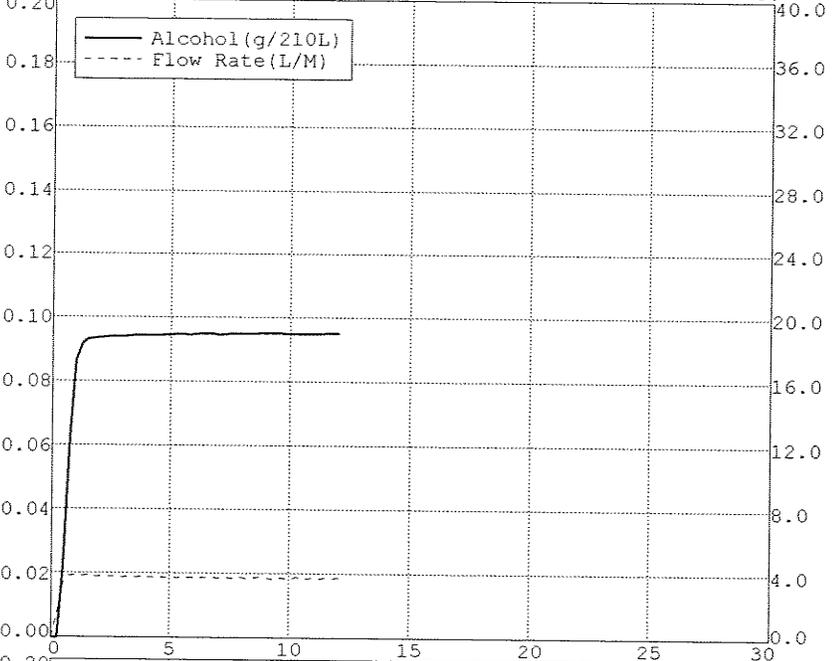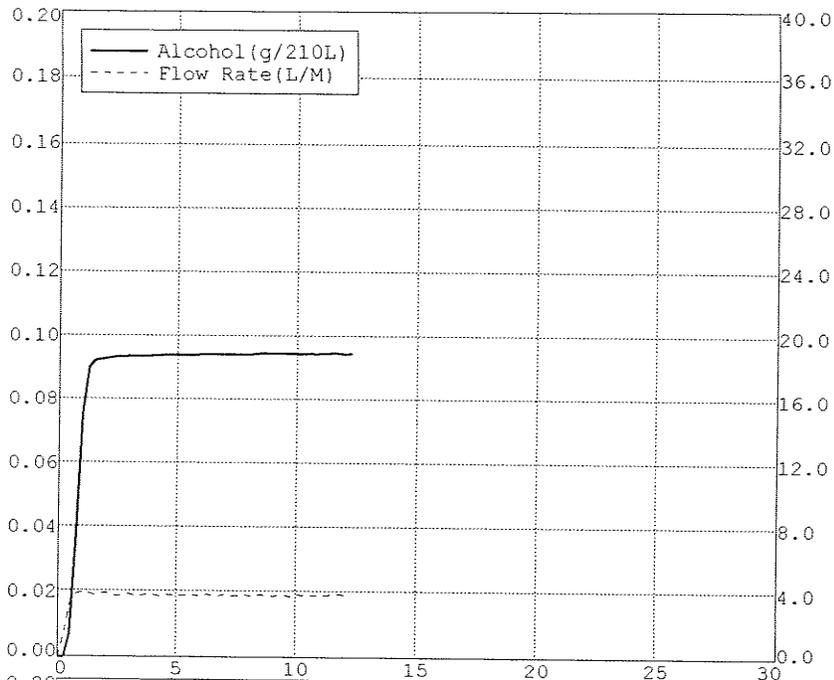

Ge. Ch. B. G. #248