

SUPERVISOR TEST




WARREN COUNTY
SHERIFF'S OFFICE
DATAMASTER dmt: 144506

Date: 10/30/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17220

Nominal = 0.10 g/210L

| | | |
|-------------------------|----------|-------|
| BLANK TEST | 0.00 | 12:14 |
| INTERNAL STANDARD | VERIFIED | 12:14 |
| REFERENCE STANDARD TEMP | 33.99c | |
| REFERENCE STANDARD | 0.09 | 12:14 |
| BLANK TEST | 0.00 | 12:15 |
| REFERENCE STANDARD TEMP | 33.98c | |
| REFERENCE STANDARD | 0.09 | 12:16 |
| BLANK TEST | 0.00 | 12:16 |
| REFERENCE STANDARD TEMP | 33.97c | |
| REFERENCE STANDARD | 0.09 | 12:17 |
| BLANK TEST | 0.00 | 12:18 |

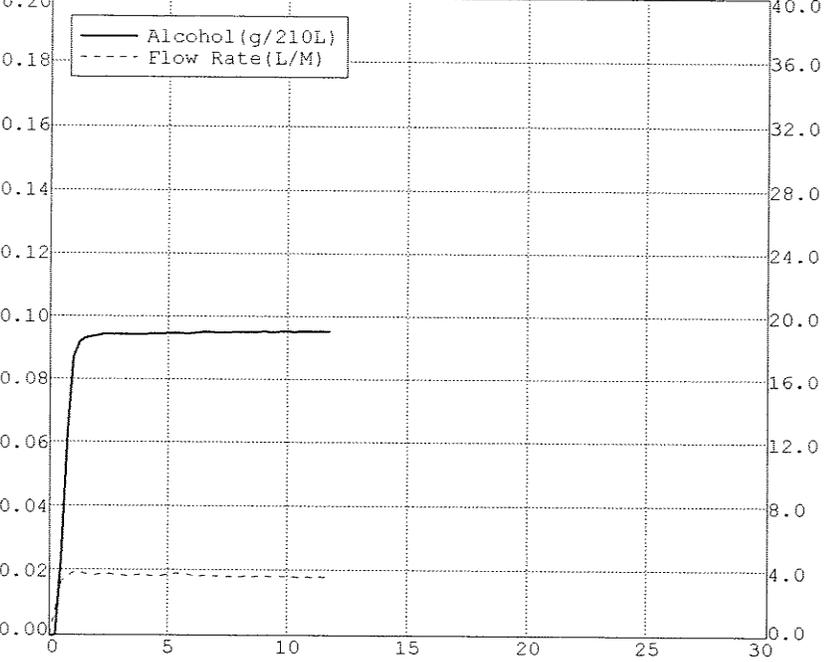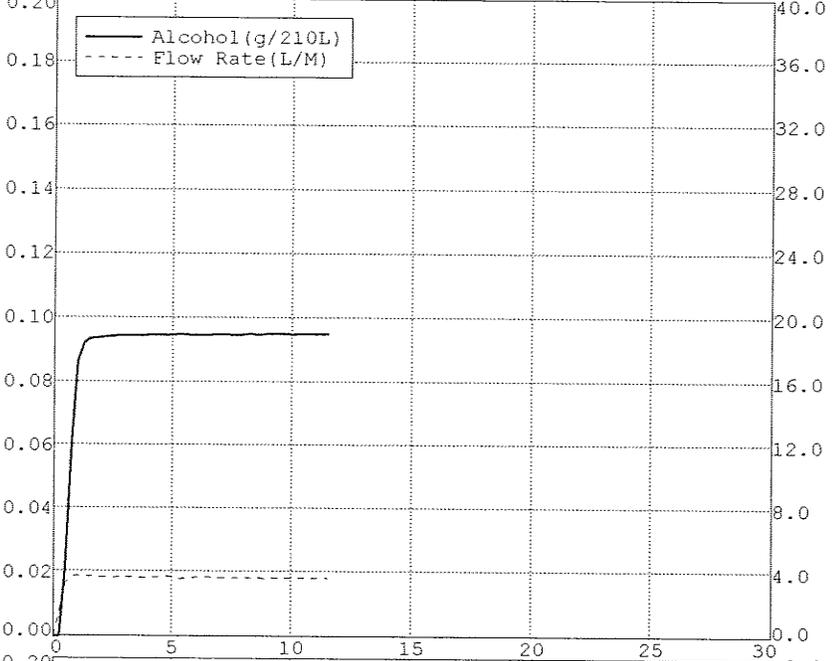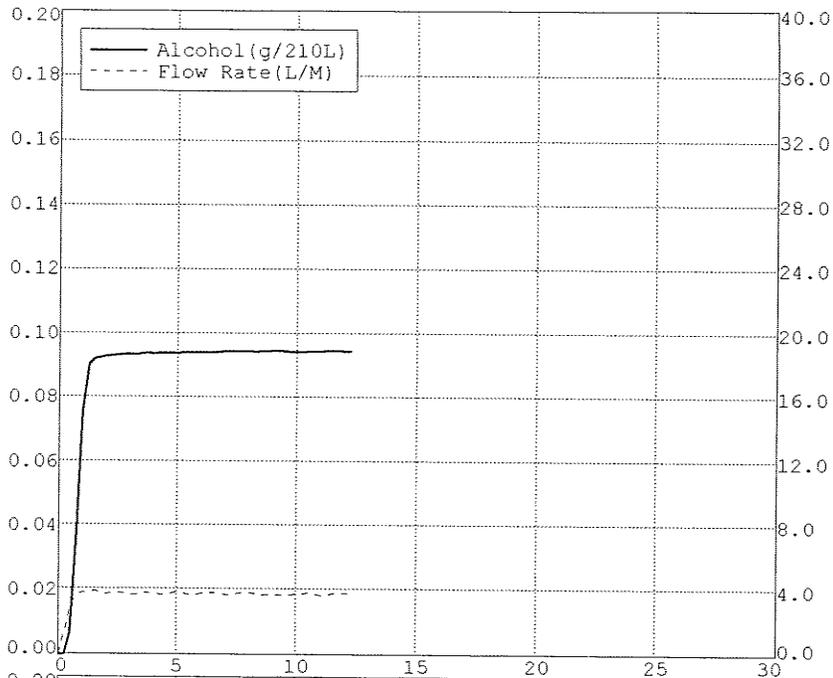

Charles B. Geisler #241