

SUPERVISOR TEST




WARREN COUNTY  
SHERIFF'S OFFICE  
DATAMASTER dmt: 144506

Date: 11/07/2017

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17220

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:32
INTERNAL STANDARD	VERIFIED	11:32
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	11:32
BLANK TEST	0.00	11:33
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	11:33
BLANK TEST	0.00	11:34
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	11:34
BLANK TEST	0.00	11:35

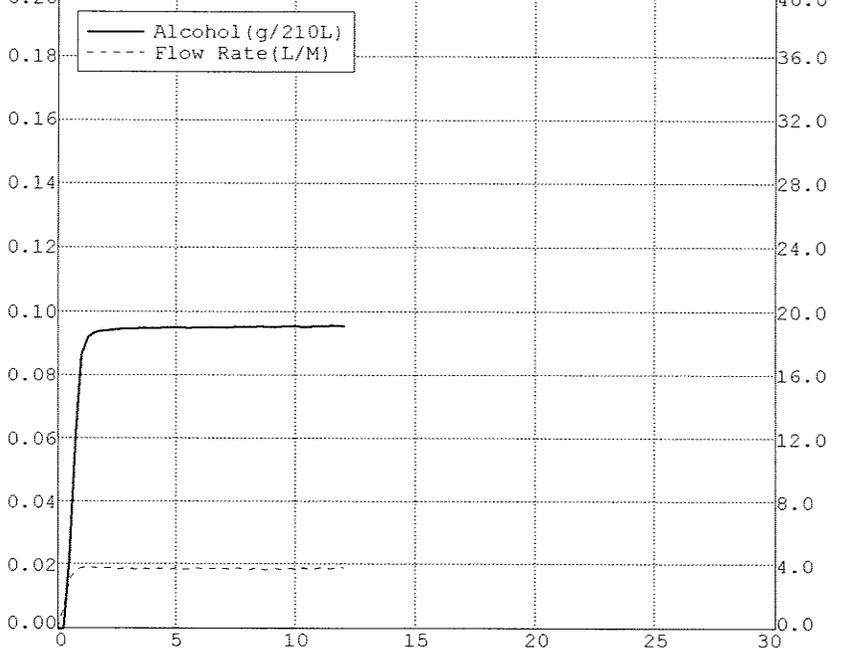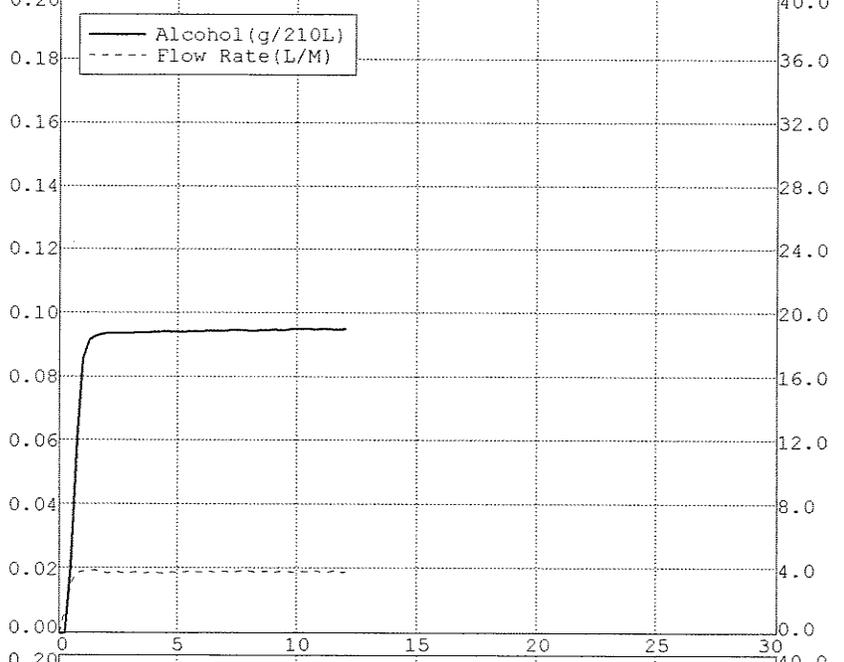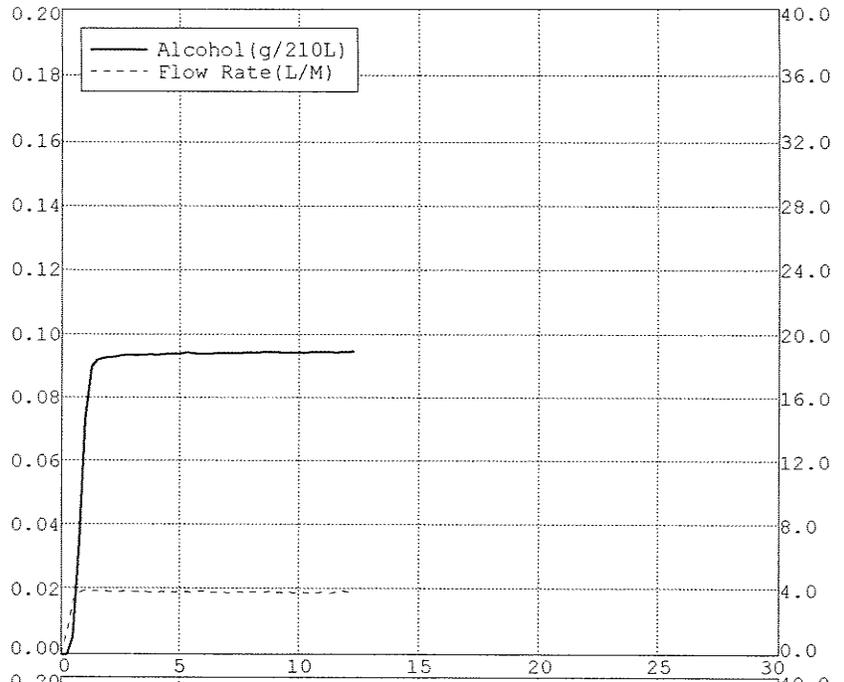

*Charles B. Geisler* #221