

SUPERVISOR TEST




WARREN COUNTY
 SHERRIF'S OFFICE
 DATAMASTER dmt: 144506

Date: 11/20/2017

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 17220

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:02
INTERNAL STANDARD	VERIFIED	03:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:02
BLANK TEST	0.00	03:03
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	03:03
BLANK TEST	0.00	03:04
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:05
BLANK TEST	0.00	03:05

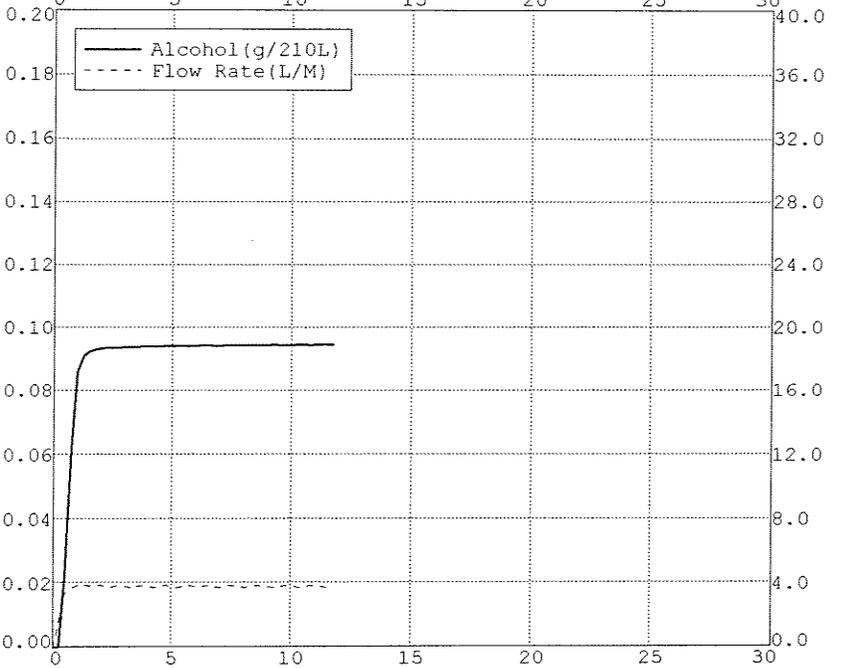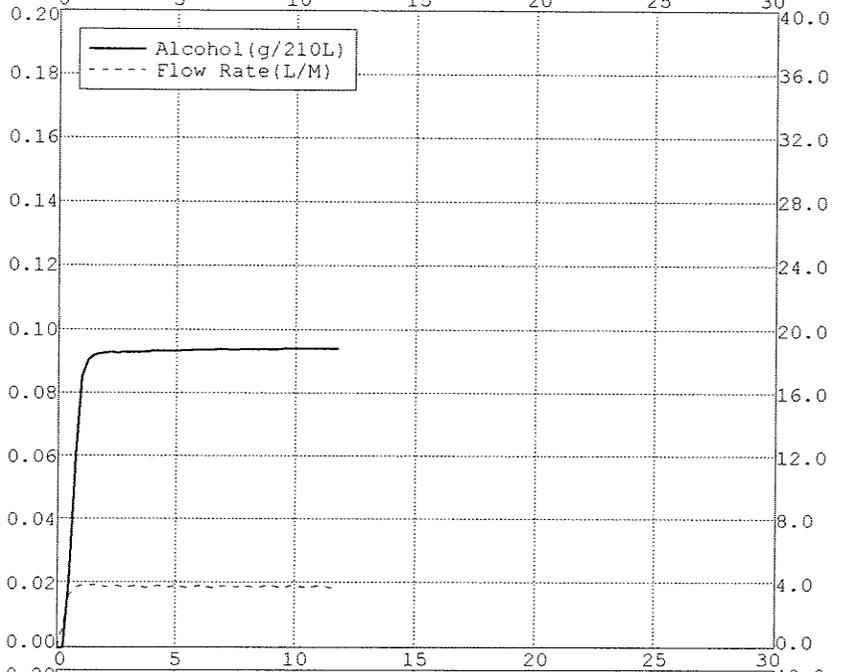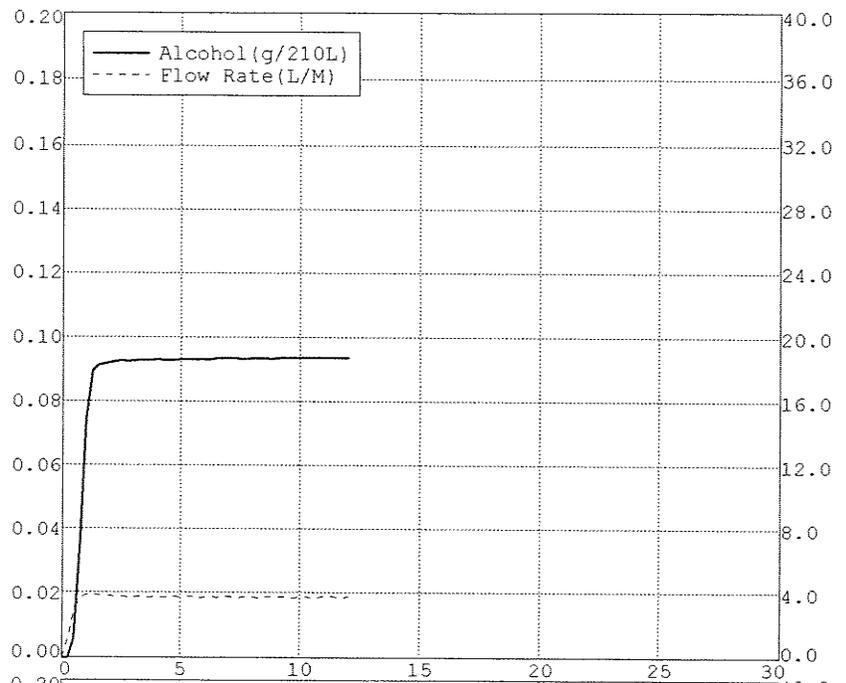

Charles B Geisler #244