

SUPERVISOR TEST




WARREN COUNTY
SHERRIF'S OFFICE
DATAMASTER dmt: 144506

Date: 12/08/2017

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17310

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:02
INTERNAL STANDARD	VERIFIED	00:02
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	00:03
BLANK TEST	0.00	00:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	00:04
BLANK TEST	0.00	00:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:05
BLANK TEST	0.00	00:06

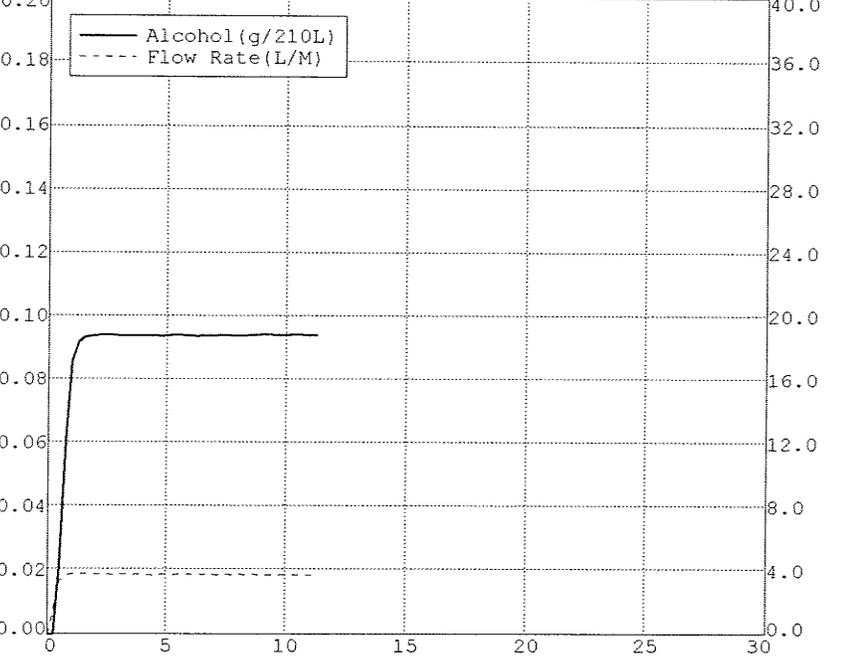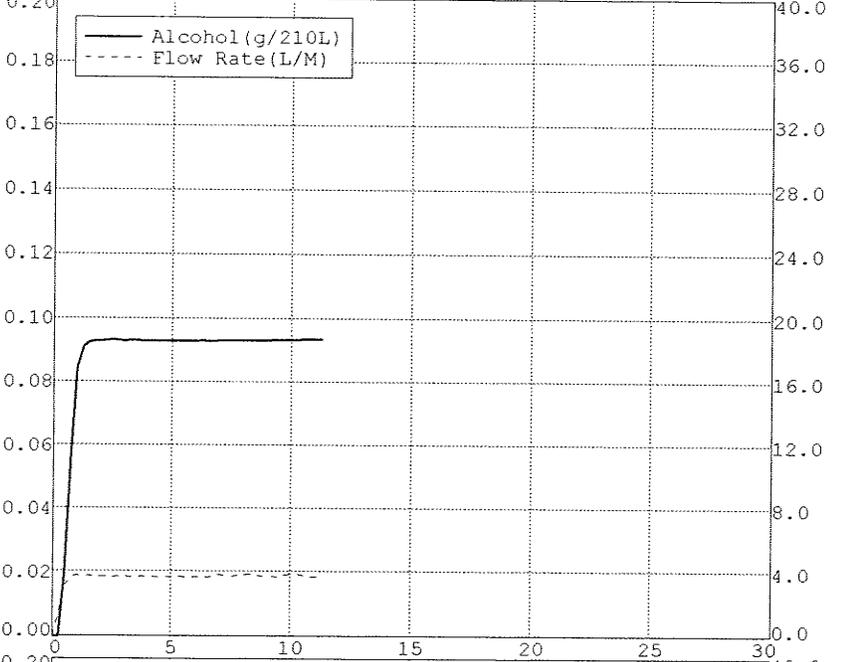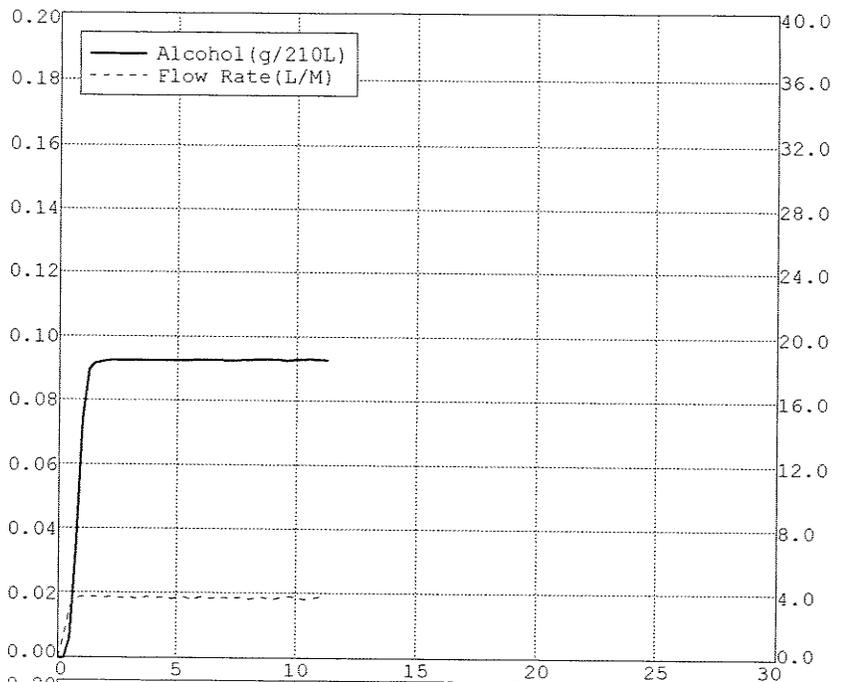

Charles B. Geisler #248