

SUPERVISOR TEST




WARREN COUNTY
 SHERRIF'S OFFICE
 DATAMASTER dmt: 144506

Date: 12/16/2017

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 17310

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:06
INTERNAL STANDARD	VERIFIED	03:06
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	03:06
BLANK TEST	0.00	03:07
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:07
BLANK TEST	0.00	03:08
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	03:08
BLANK TEST	0.00	03:09

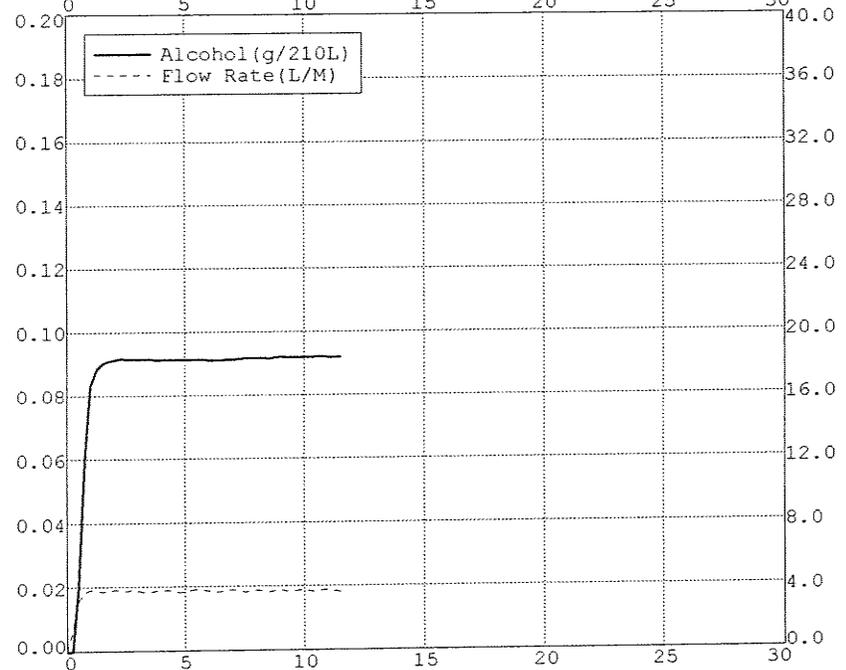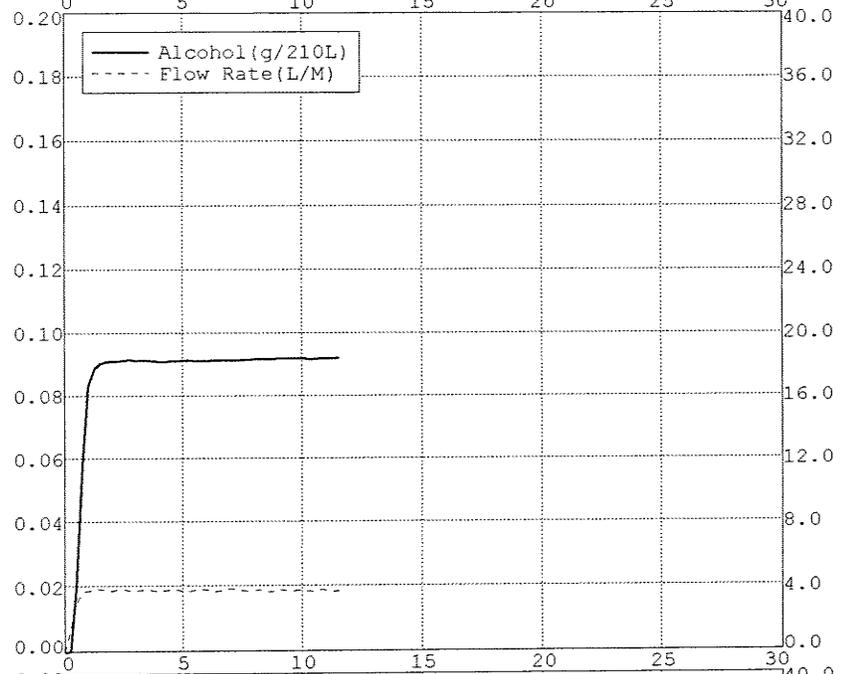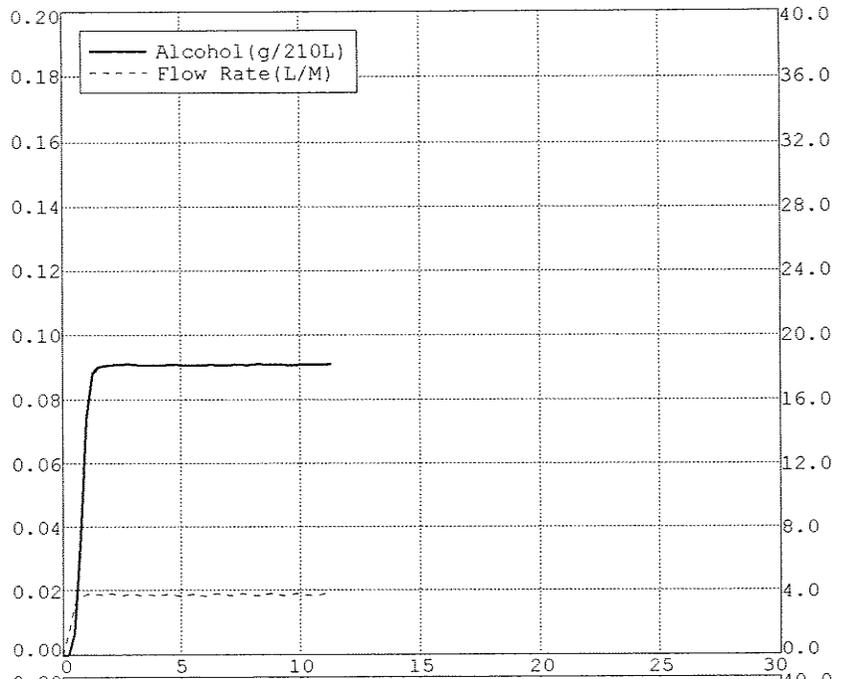

Charles B. Geisler #245