

SUPERVISOR TEST




WARREN COUNTY  
 SHERRIF'S OFFICE  
 DATAMASTER dmt: 144506

Date: 12/25/2017

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 17310

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:55
INTERNAL STANDARD	VERIFIED	22:56
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.08	22:56
BLANK TEST	0.00	22:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:57
BLANK TEST	0.00	22:58
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.09	22:58
BLANK TEST	0.00	22:59

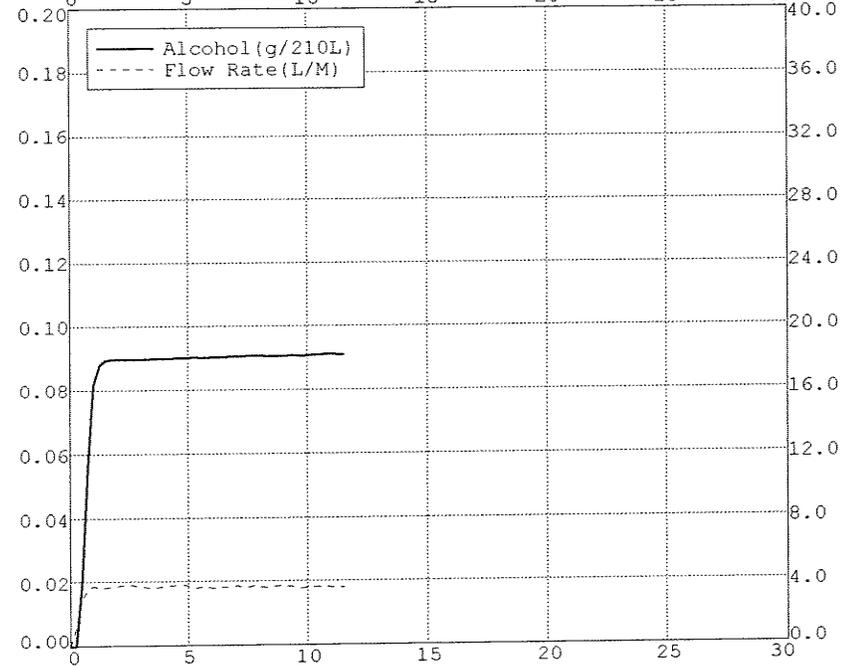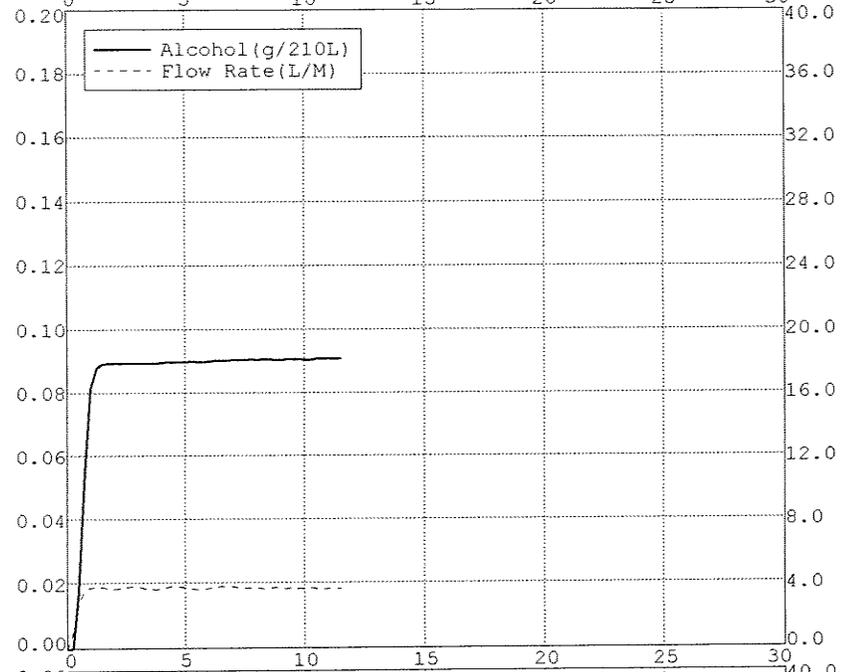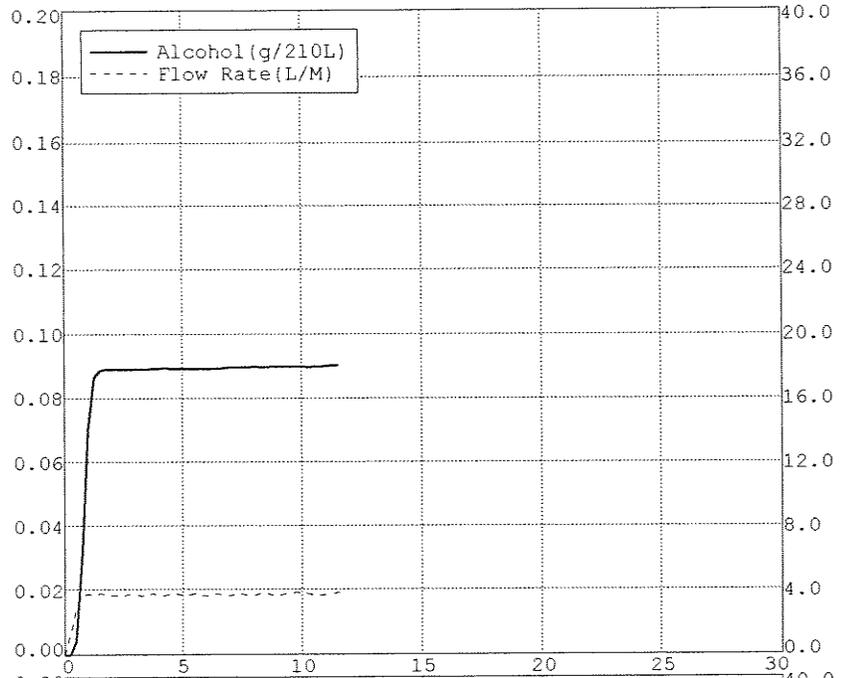

*Ge. C. B. Geisler #2018*

SUPERVISOR TEST




WARREN COUNTY  
SHERRIF'S OFFICE  
DATAMASTER dmt: 144506

Date: 12/25/2017

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17310

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:02
INTERNAL STANDARD	VERIFIED	23:02
REFERENCE STANDARD TEMP	33.96c	
REFERENCE STANDARD	0.09	23:03
BLANK TEST	0.00	23:04
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	23:04
BLANK TEST	0.00	23:05
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.09	23:05
BLANK TEST	0.00	23:06

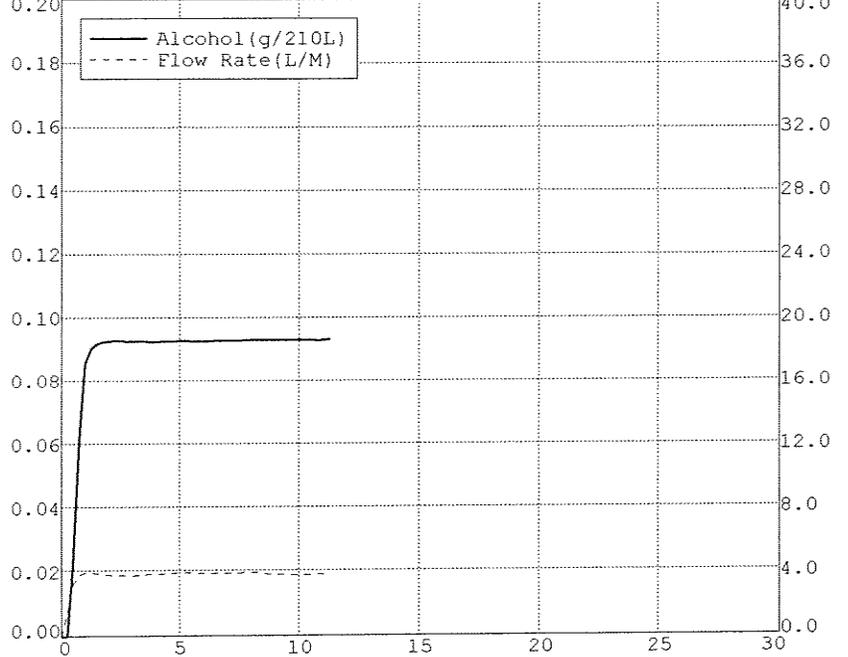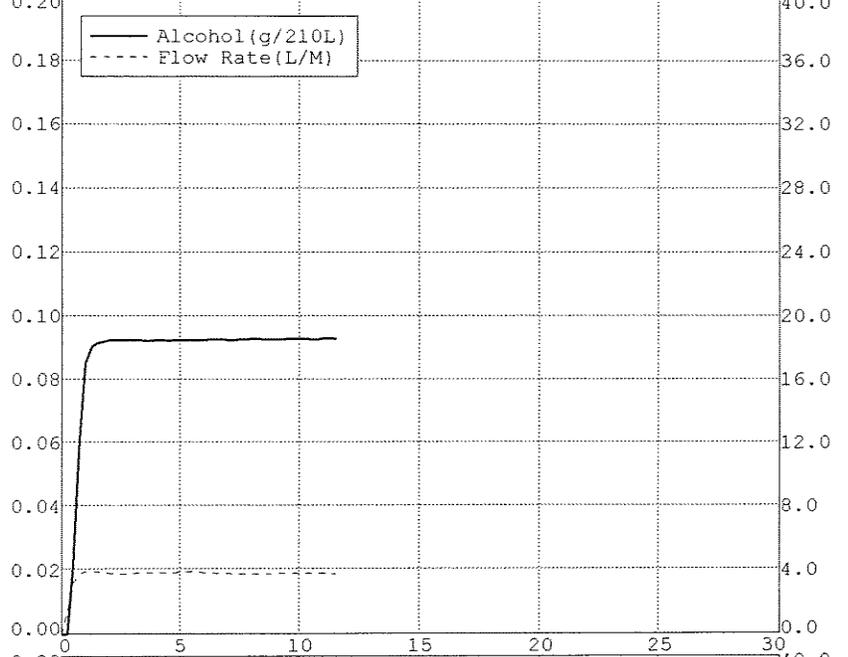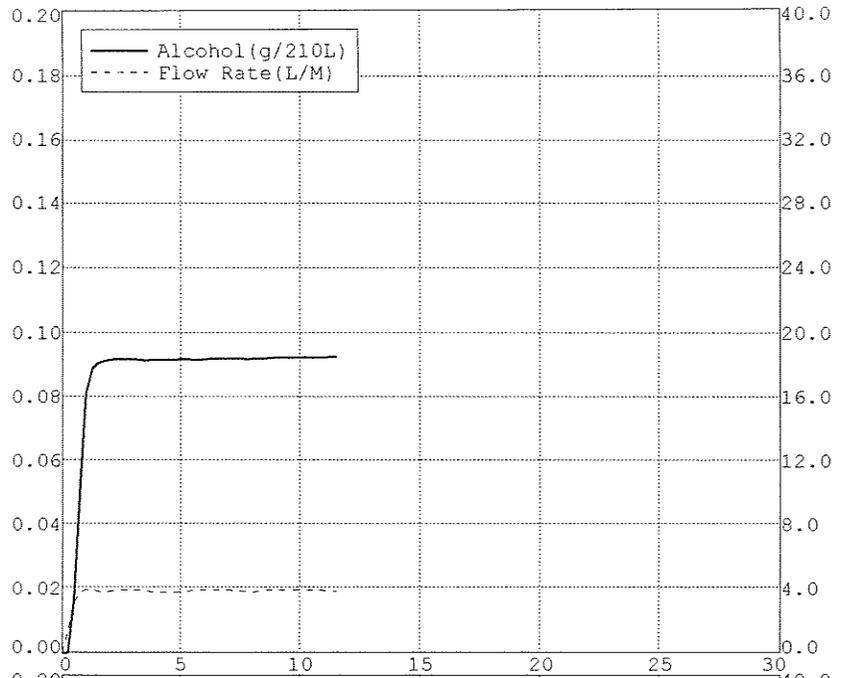

*Charles B Geisler #211*