

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 01/13/2018

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17310

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:34
INTERNAL STANDARD	VERIFIED	23:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:34
BLANK TEST	0.00	23:35
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	23:36
BLANK TEST	0.00	23:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:37
BLANK TEST	0.00	23:38

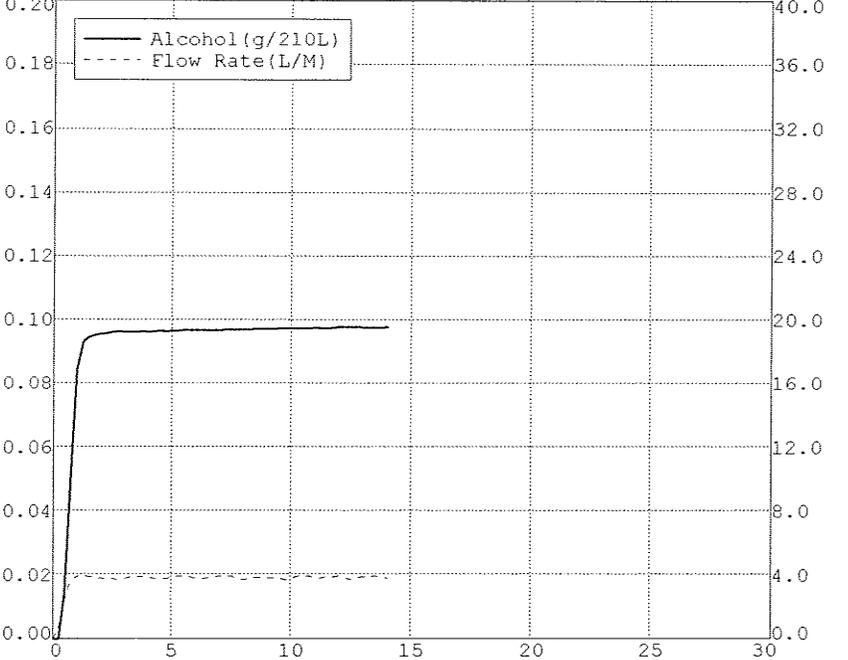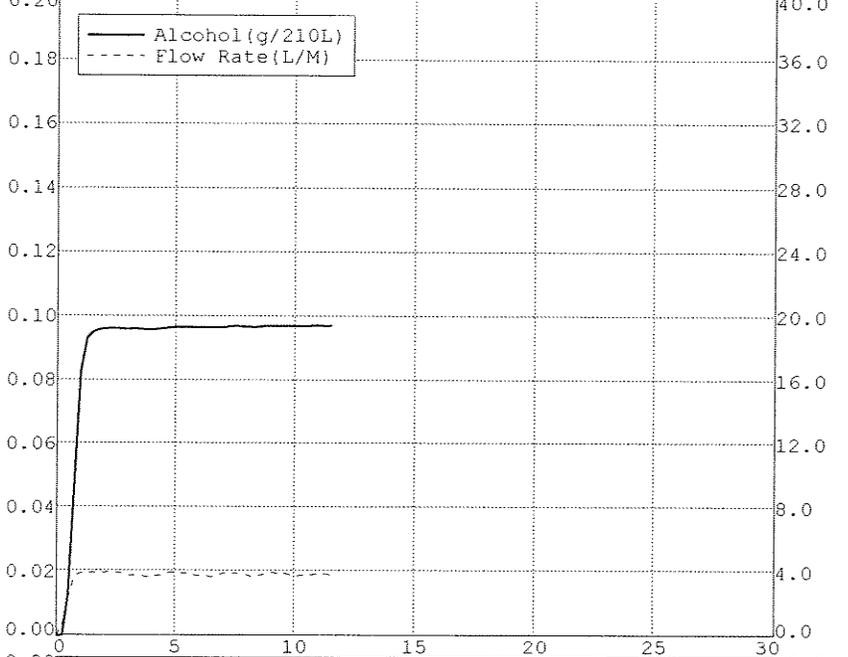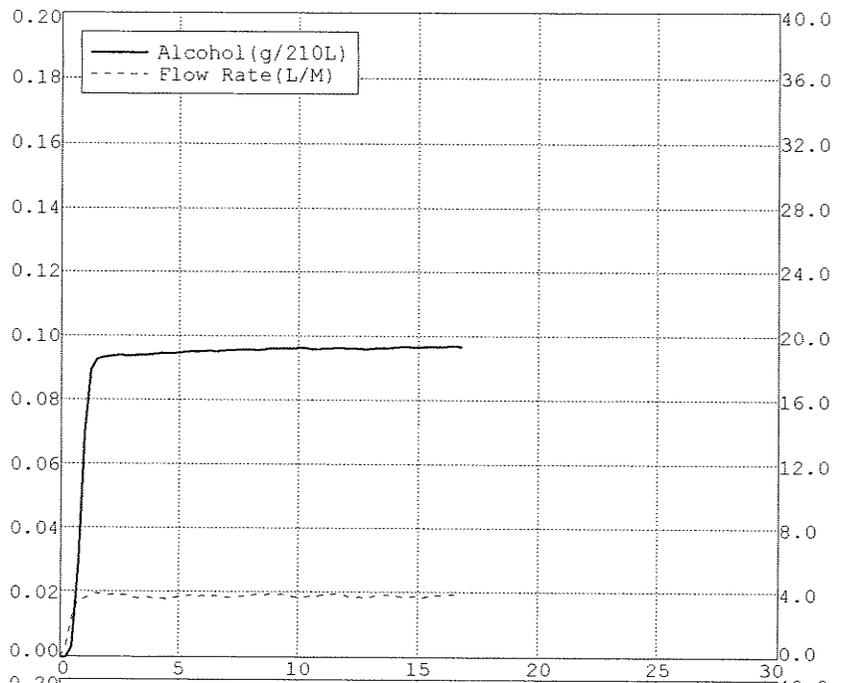

*Charles B. Geisler #245*