

SUPERVISOR TEST




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208

Date: 02/09/2018

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 17390

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:00
INTERNAL STANDARD	VERIFIED	23:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:00
BLANK TEST	0.00	23:01
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	23:02
BLANK TEST	0.00	23:03
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	23:03
BLANK TEST	0.00	23:04

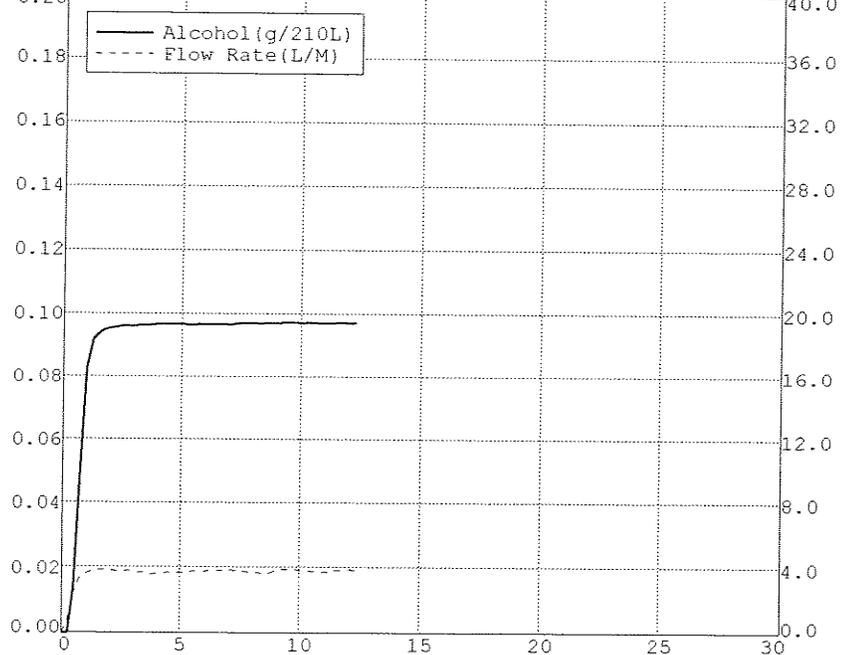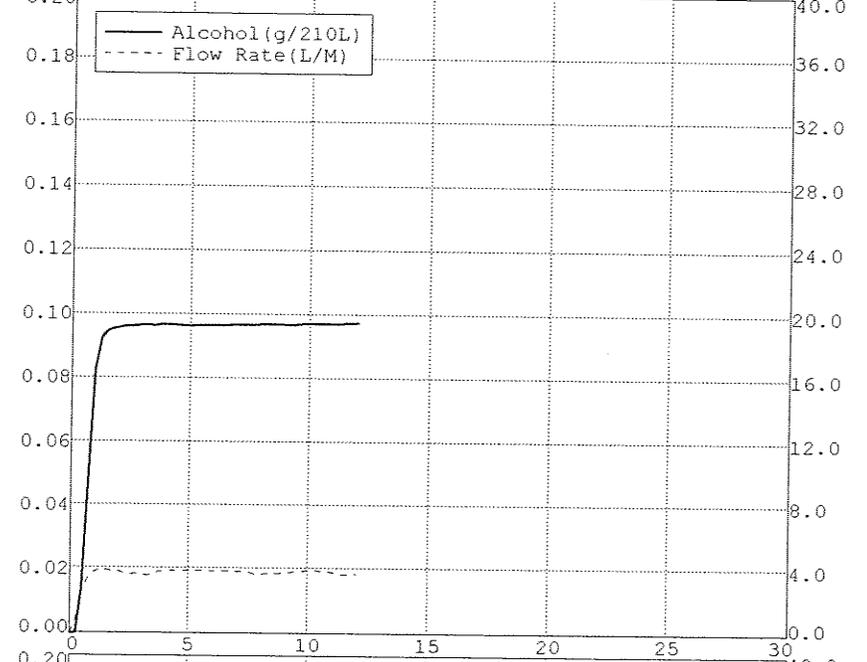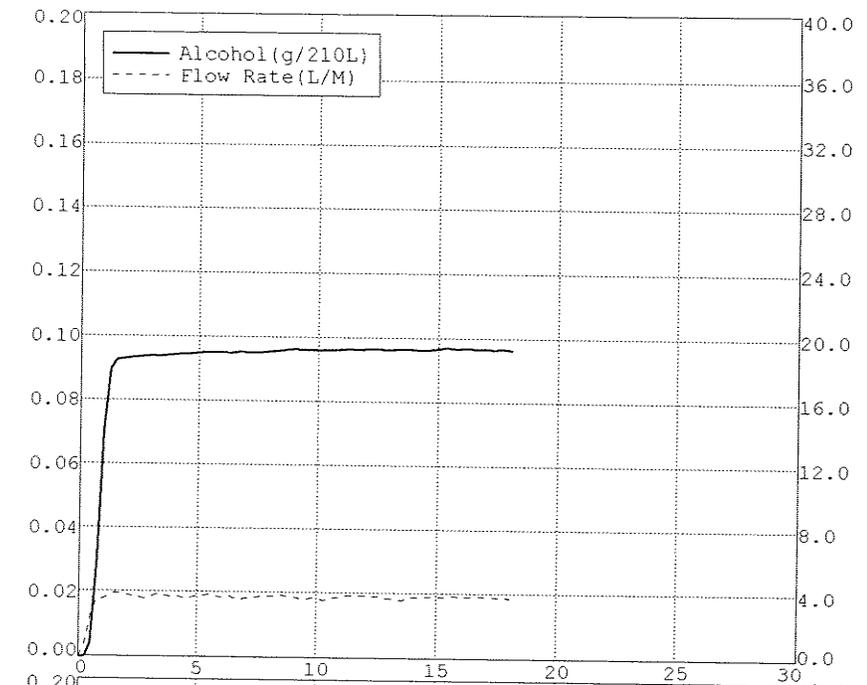

Handwritten signature: J. B. Geisler #241