

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 02/16/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17390

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:12
INTERNAL STANDARD	VERIFIED	03:13
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:13
BLANK TEST	0.00	03:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:14
BLANK TEST	0.00	03:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:16
BLANK TEST	0.00	03:17

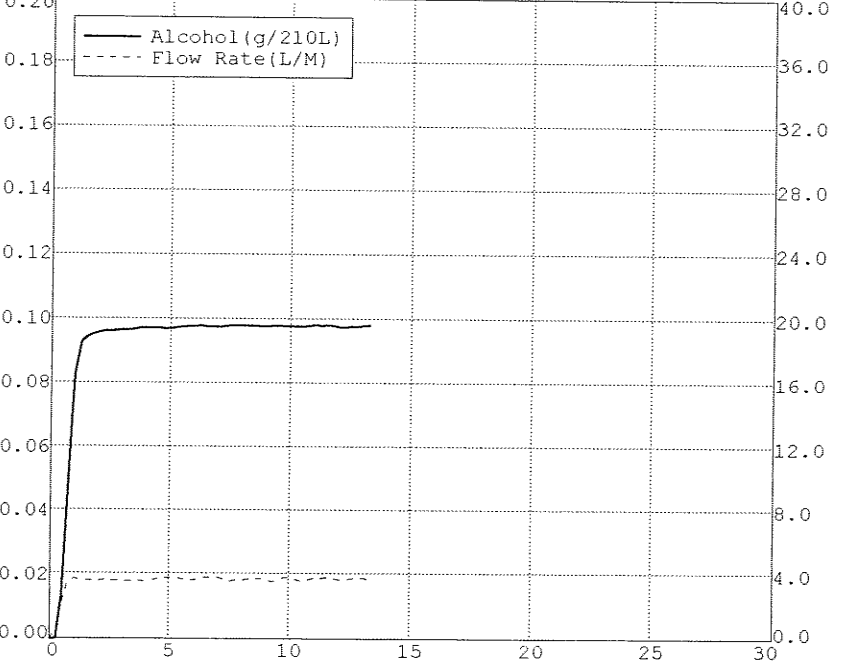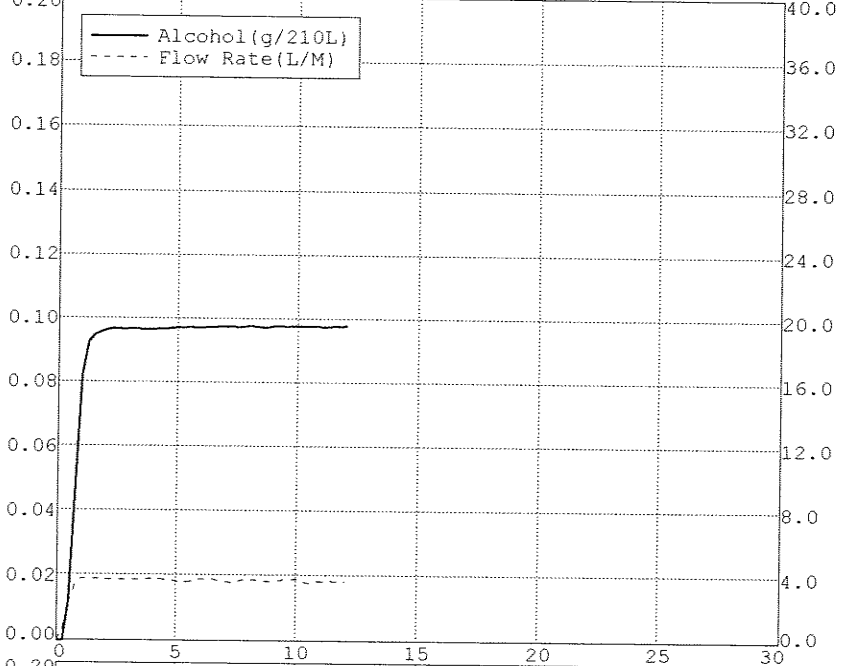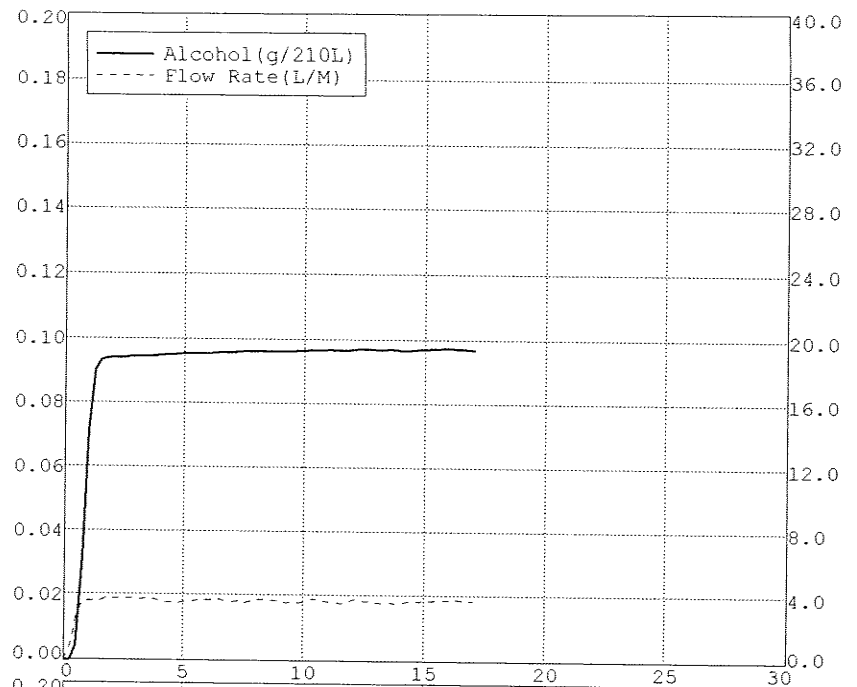

Charles B. Geisler #33757