

SUPERVISOR TEST



WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 03/07/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17390

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:29
INTERNAL STANDARD	VERIFIED	03:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	03:29
BLANK TEST	0.00	03:30
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	03:31
BLANK TEST	0.00	03:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	03:32
BLANK TEST	0.00	03:33

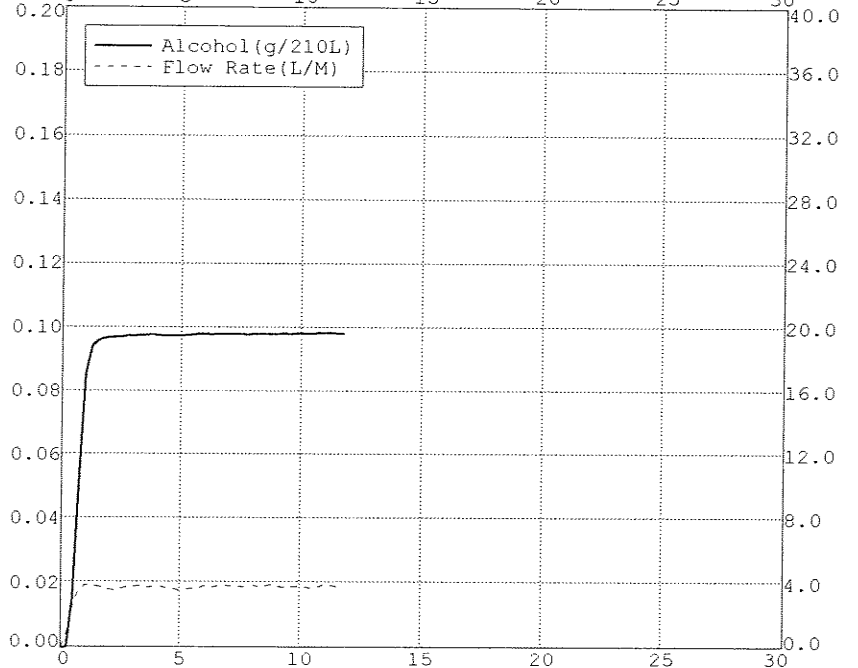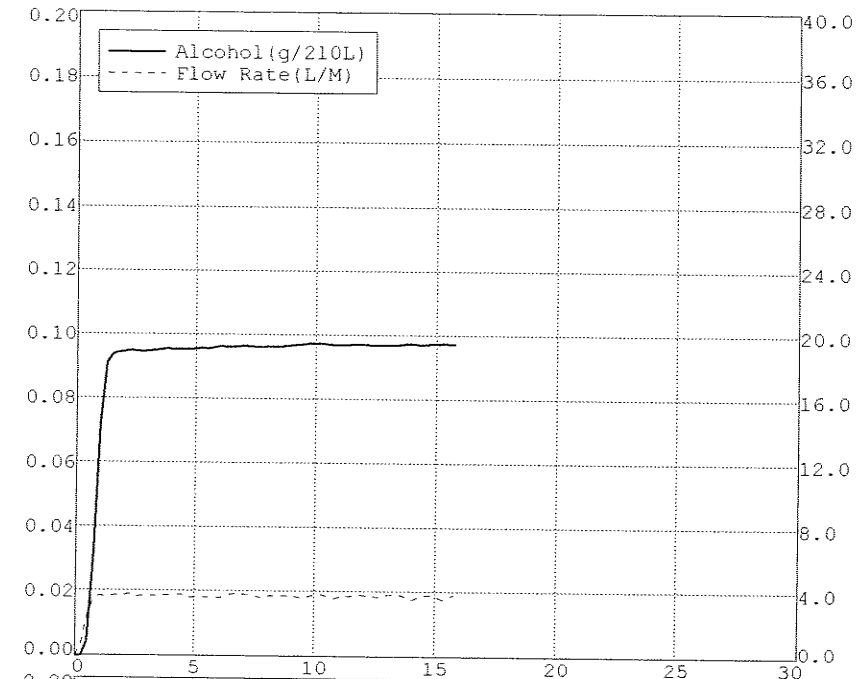

Handwritten signature: Charles B. Geisler