

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 03/15/2018

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 17390

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:56
INTERNAL STANDARD	VERIFIED	02:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:56
BLANK TEST	0.00	02:57
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	02:57
BLANK TEST	0.00	02:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	02:59
BLANK TEST	0.00	03:00

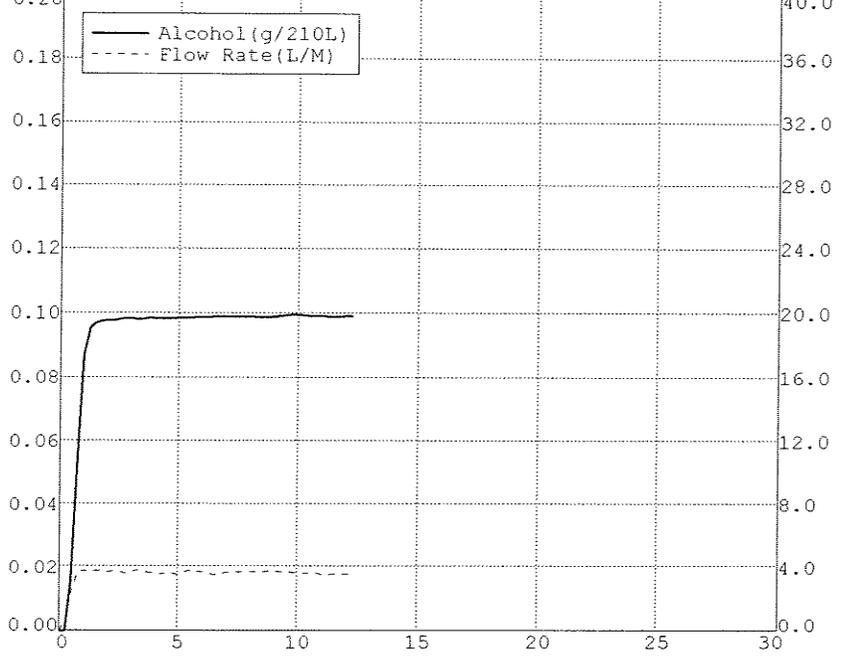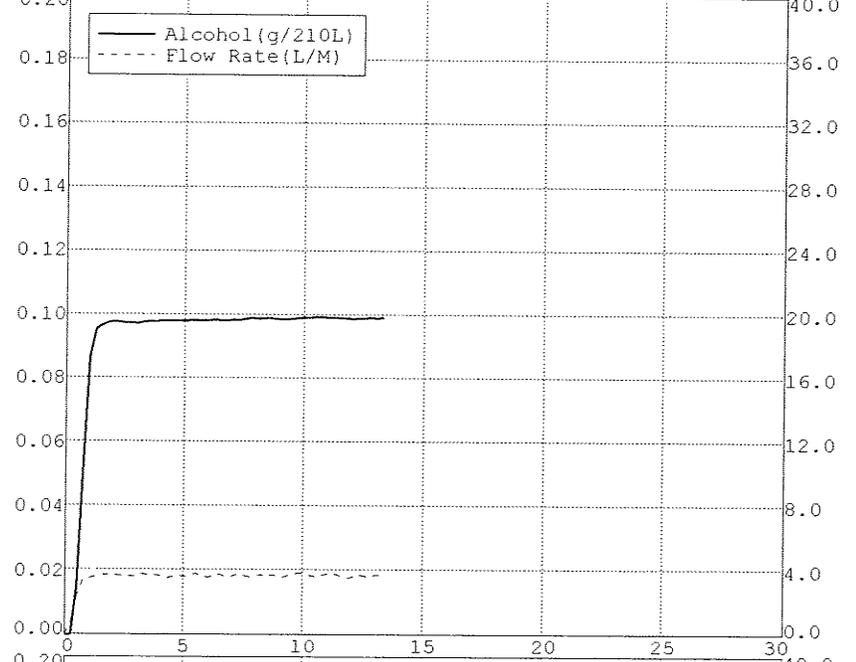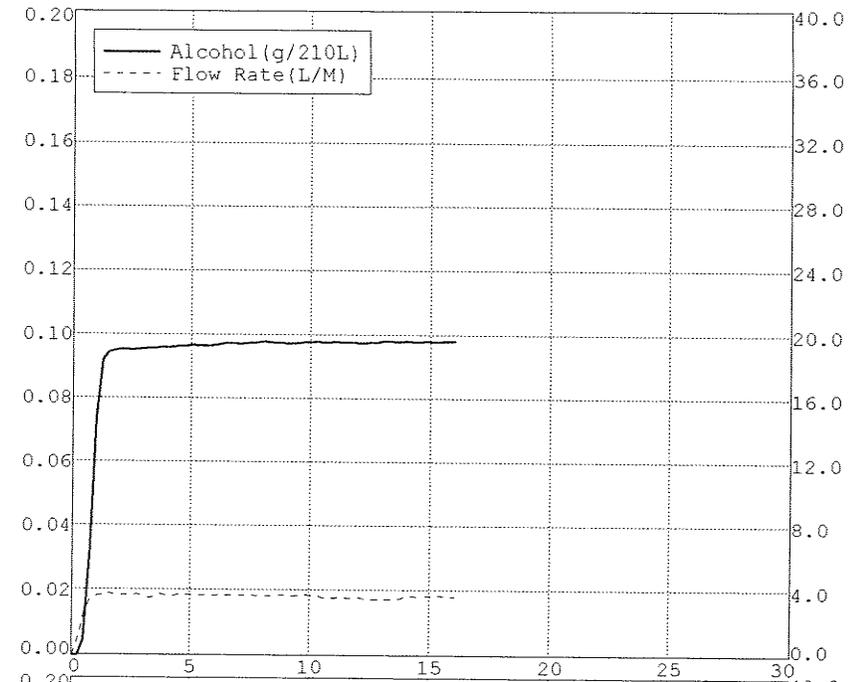

*Handwritten signature: C. B. Geisler #241*