

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 03/23/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 17390

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:55
INTERNAL STANDARD	VERIFIED	23:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:56
BLANK TEST	0.00	23:56
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	23:57
BLANK TEST	0.00	23:58
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	23:58
BLANK TEST	0.00	23:59

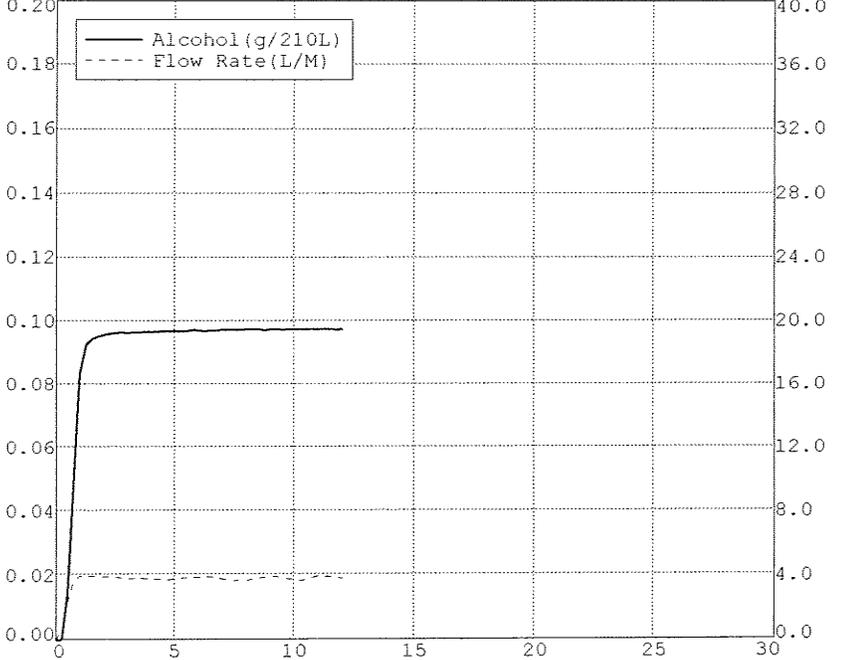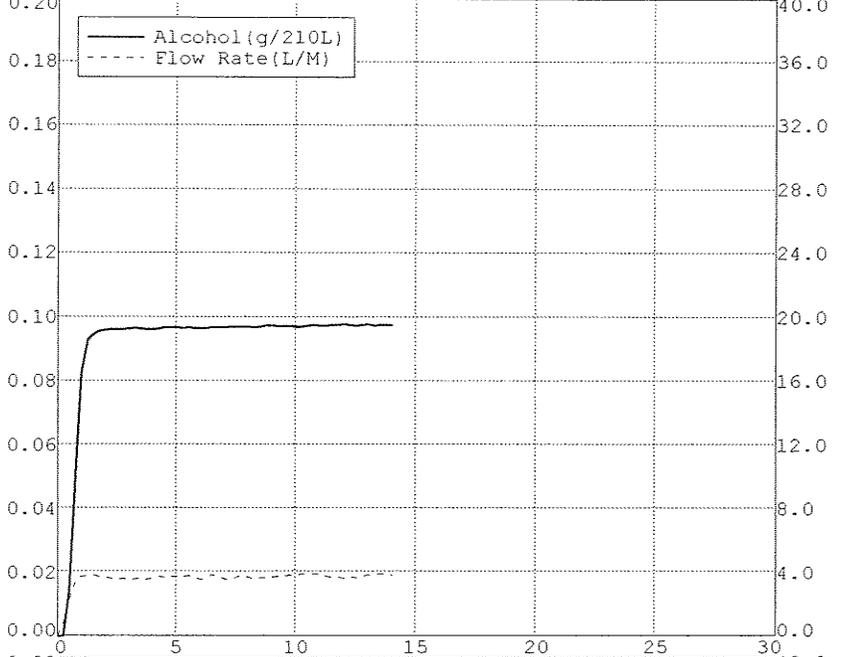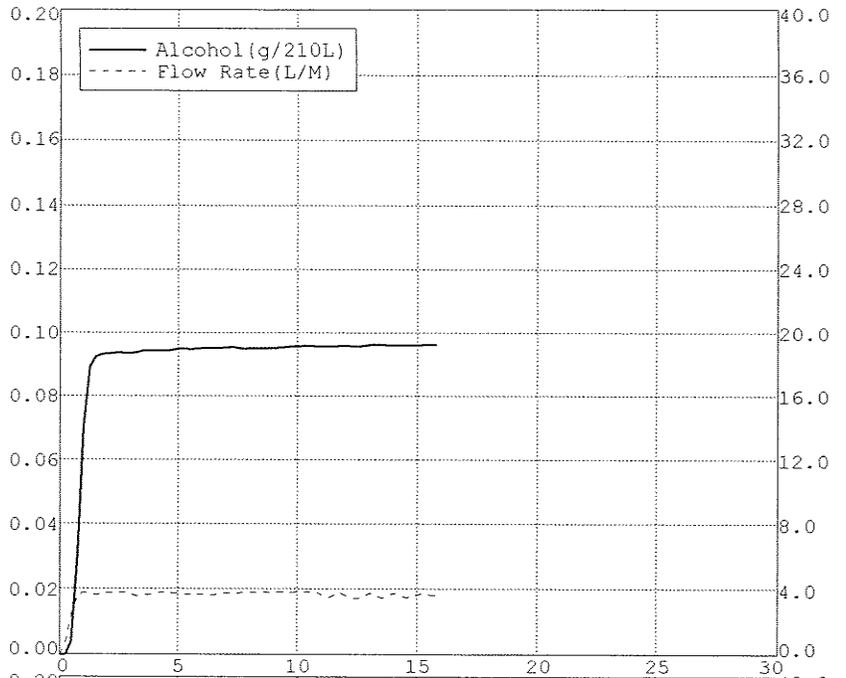

Charles B. Geisler #24