

SOLUTION CHANGE




 WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208

Date: 03/30/2018

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 18040

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:19
INTERNAL STANDARD	VERIFIED	05:19
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	05:19
BLANK TEST	0.00	05:20
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:20
BLANK TEST	0.00	05:21
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	05:22
BLANK TEST	0.00	05:23

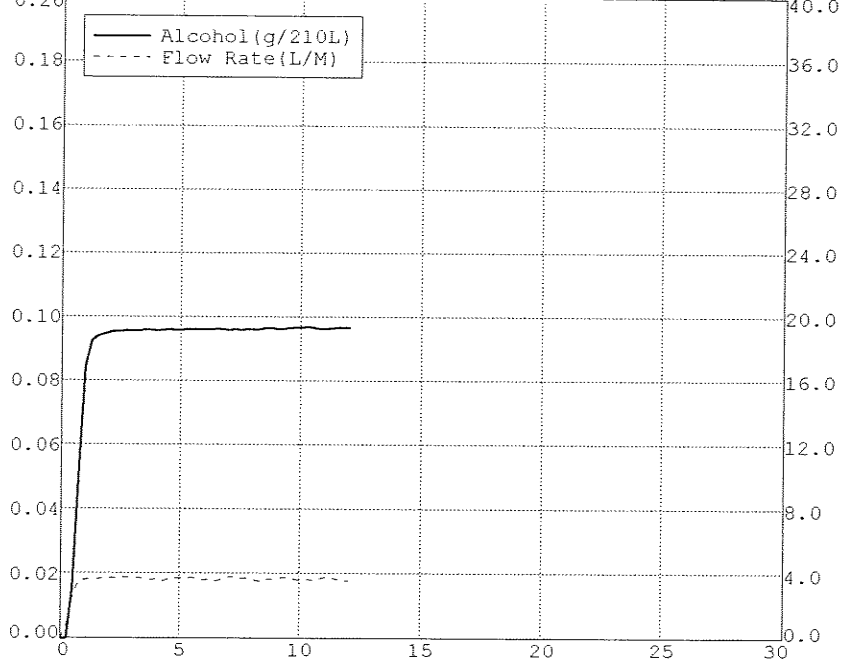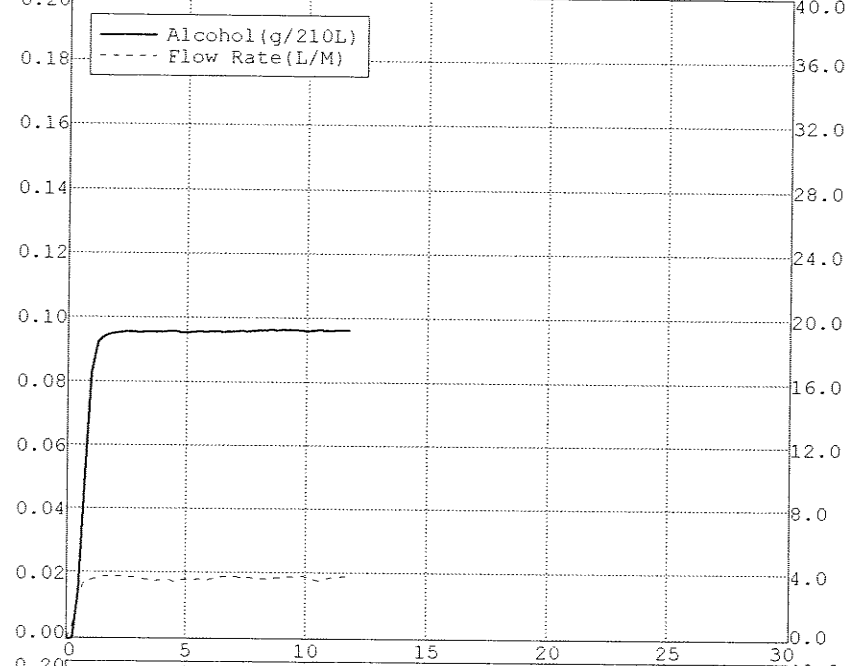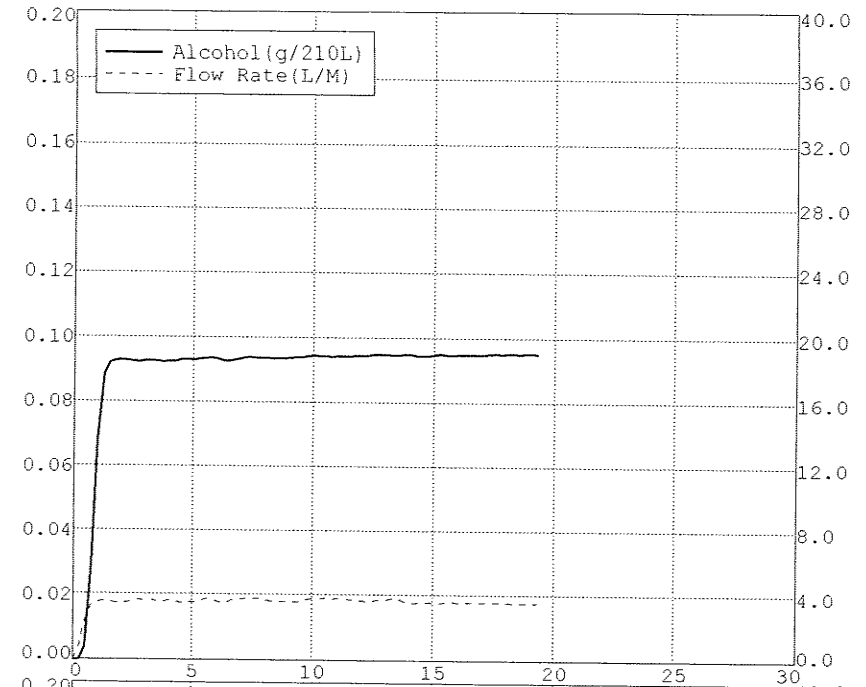

Charles B Geisler #246