

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 04/13/2018

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18040

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:24
INTERNAL STANDARD	VERIFIED	04:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	04:24
BLANK TEST	0.00	04:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	04:26
BLANK TEST	0.00	04:26
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	04:27
BLANK TEST	0.00	04:28

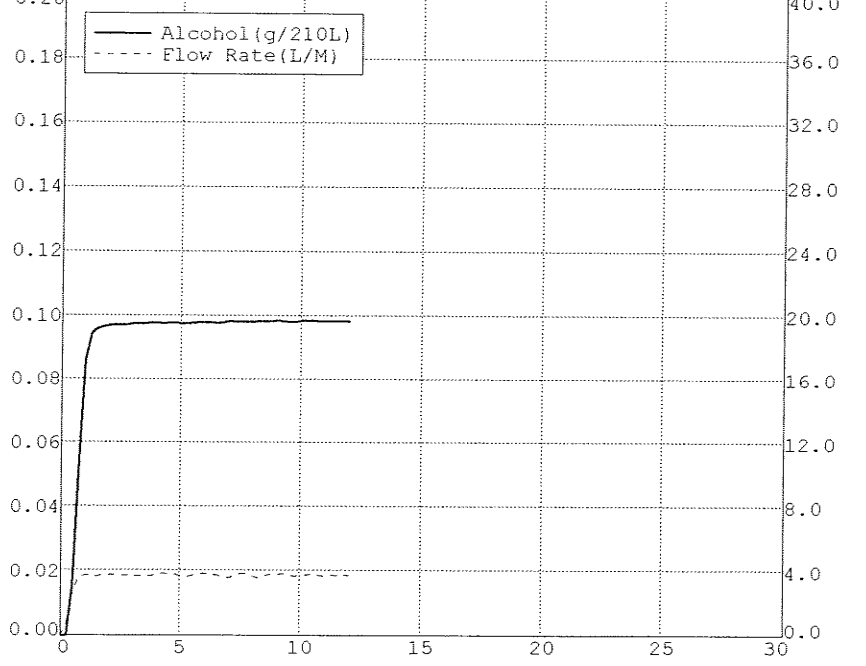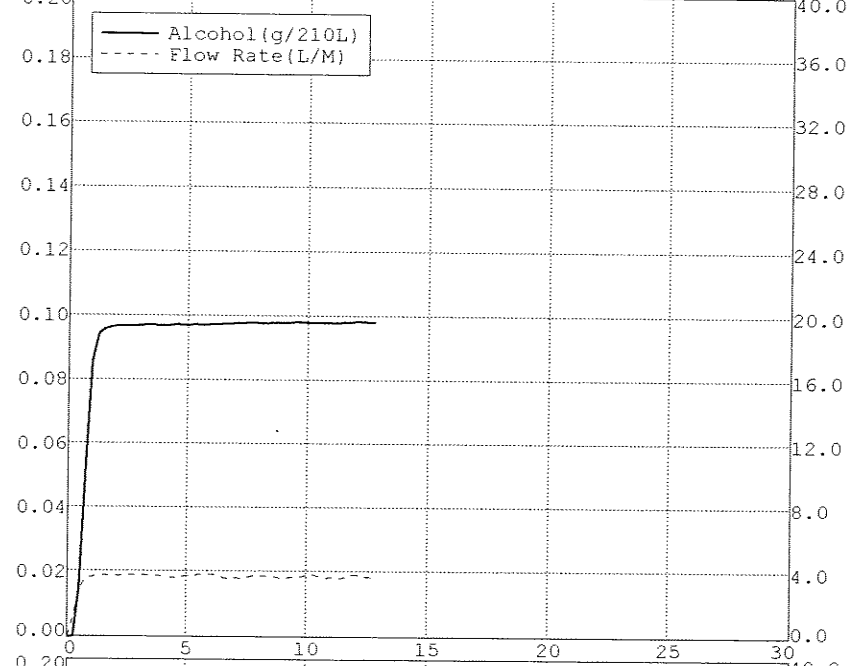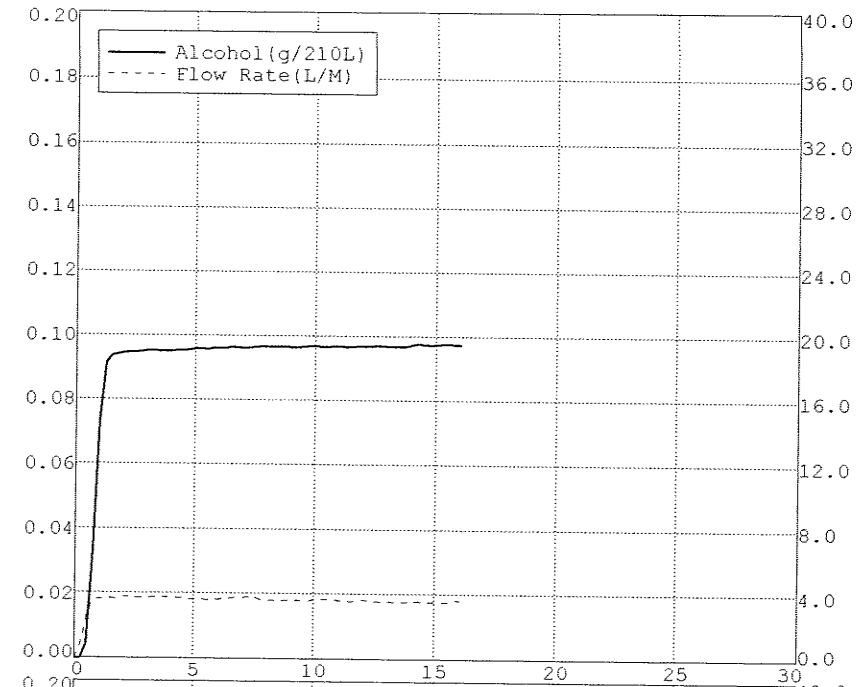

*Charles B. Geisler* #224