

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 04/21/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18040

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:33
INTERNAL STANDARD	VERIFIED	23:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	23:34
BLANK TEST	0.00	23:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	23:35
BLANK TEST	0.00	23:36
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	23:37
BLANK TEST	0.00	23:38

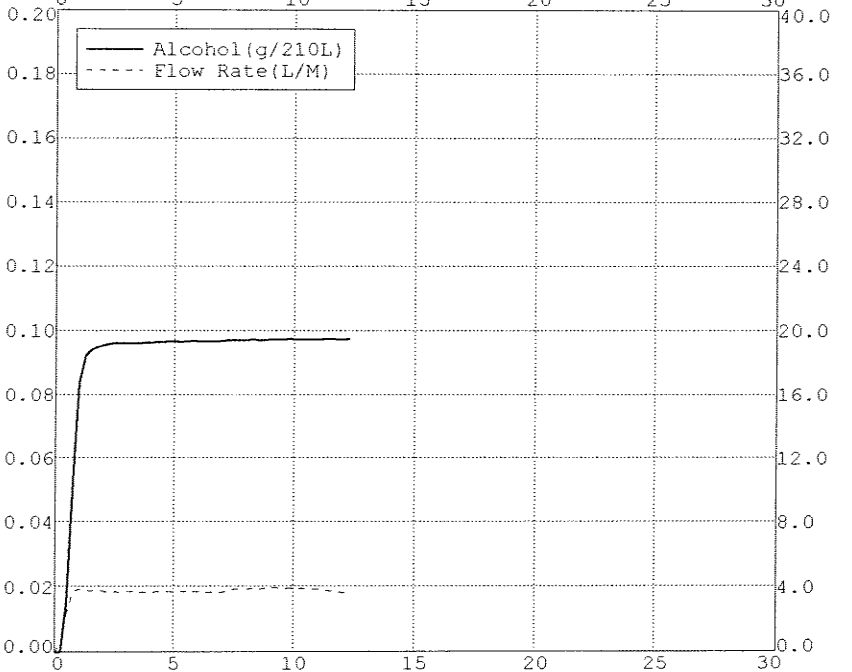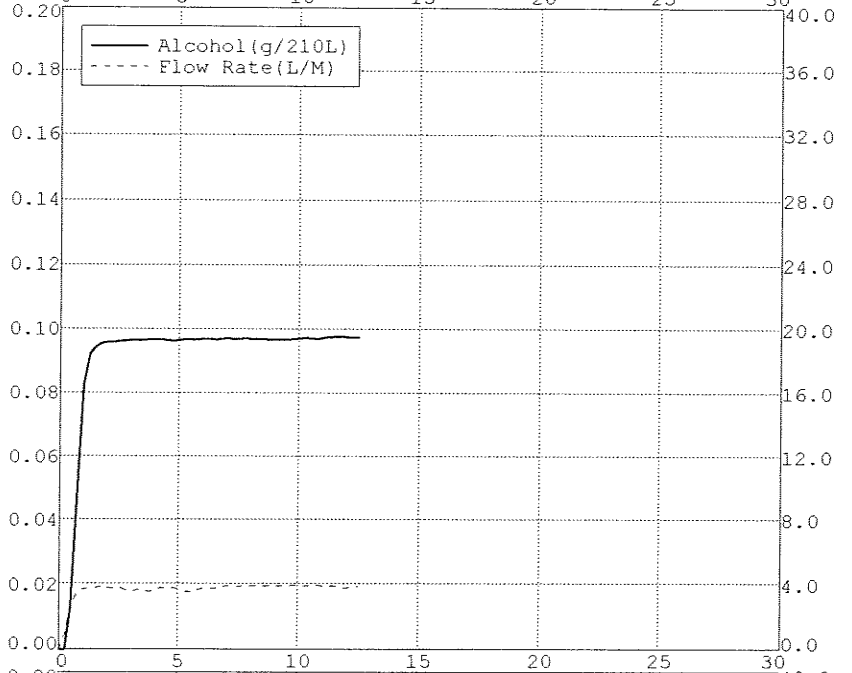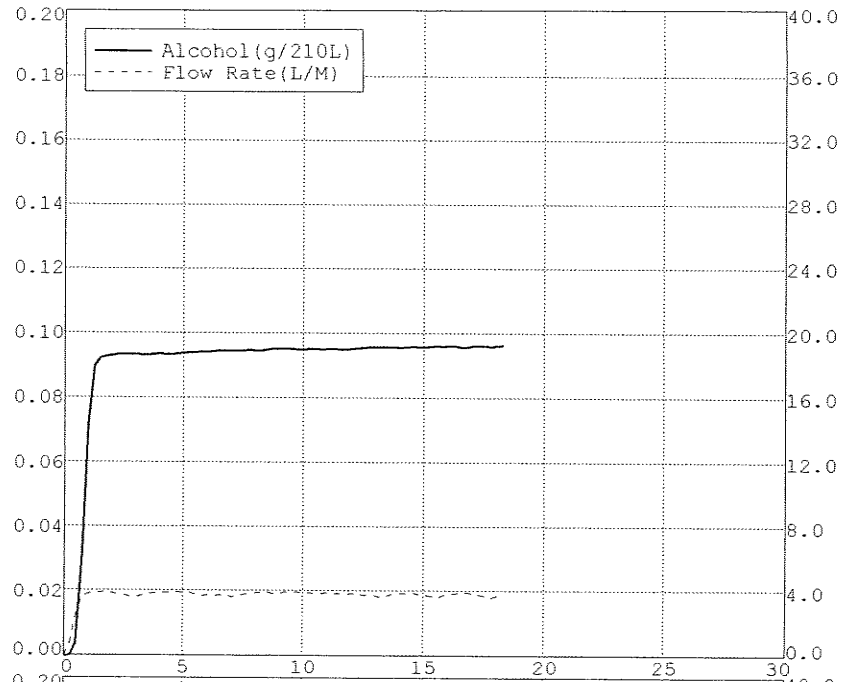

Charles B. Geisler #245