

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 04/28/2018

OPERATOR NAME:
J T COON
Permit #: 36043
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18040

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:15
INTERNAL STANDARD	VERIFIED	20:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	20:16
BLANK TEST	0.00	20:17
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	20:17
BLANK TEST	0.00	20:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	20:19
BLANK TEST	0.00	20:19

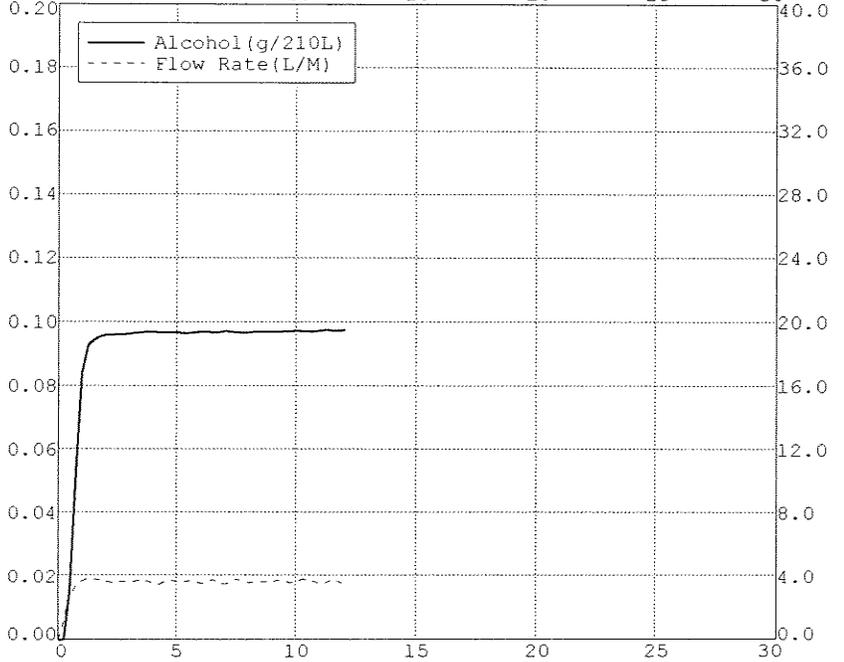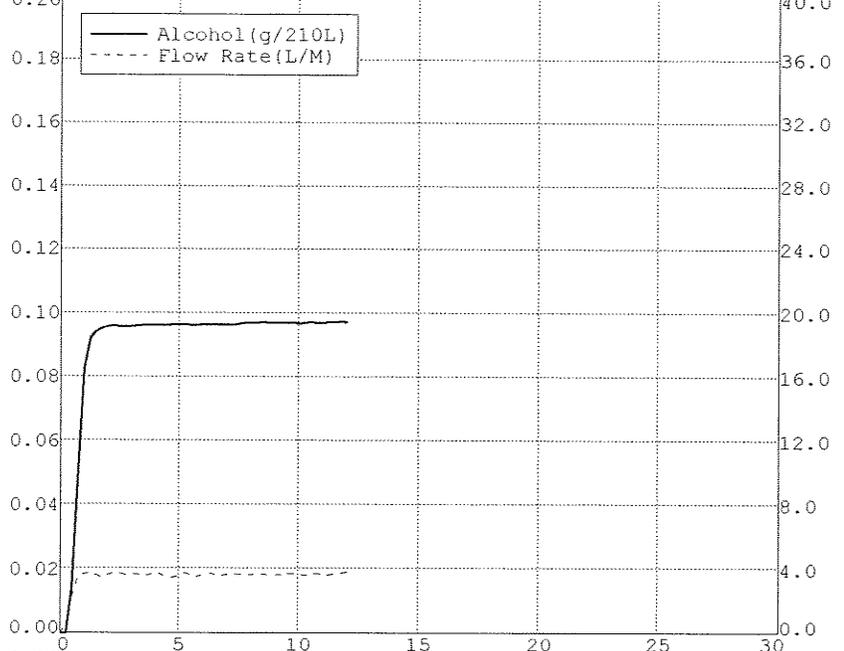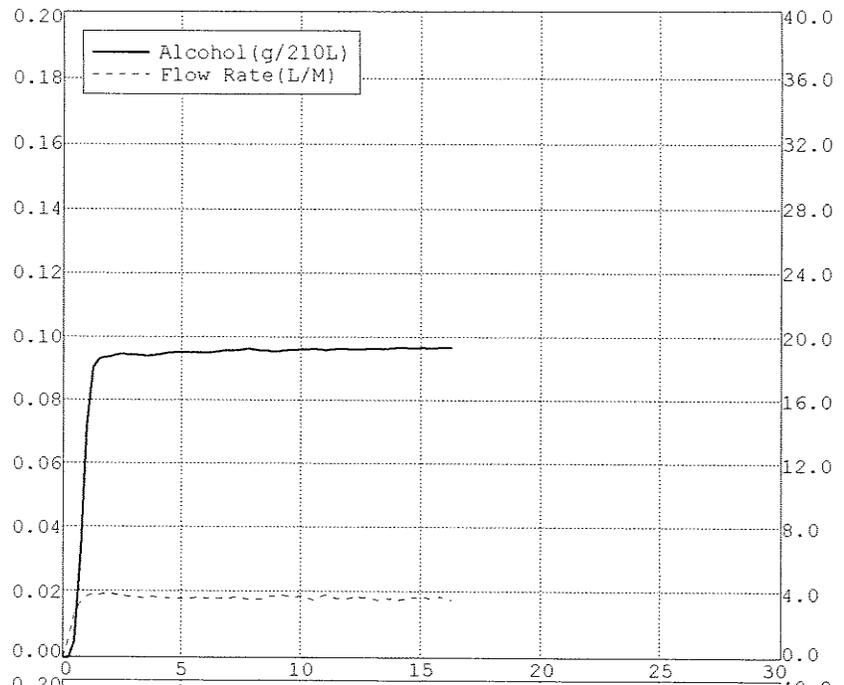

J.T. Coon