

SUPERVISOR TEST

WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 105208




Date: 05/09/2018

OPERATOR NAME:  
 RYAN C SCHROECK  
 Permit #: 41316  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 18040

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:39
INTERNAL STANDARD	VERIFIED	11:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:39
BLANK TEST	0.00	11:40
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	11:40
BLANK TEST	0.00	11:41
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	11:42
BLANK TEST	0.00	11:43

*PO [Signature]*

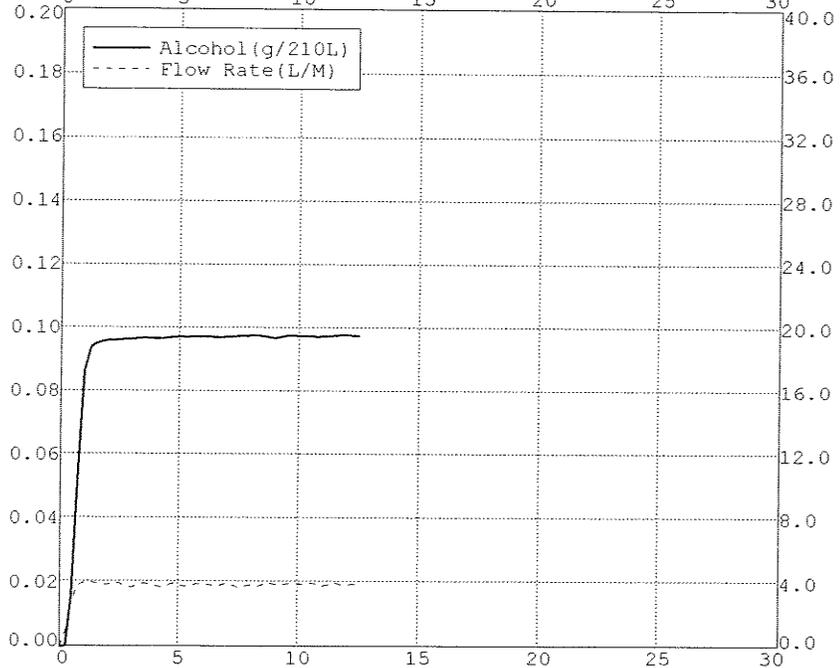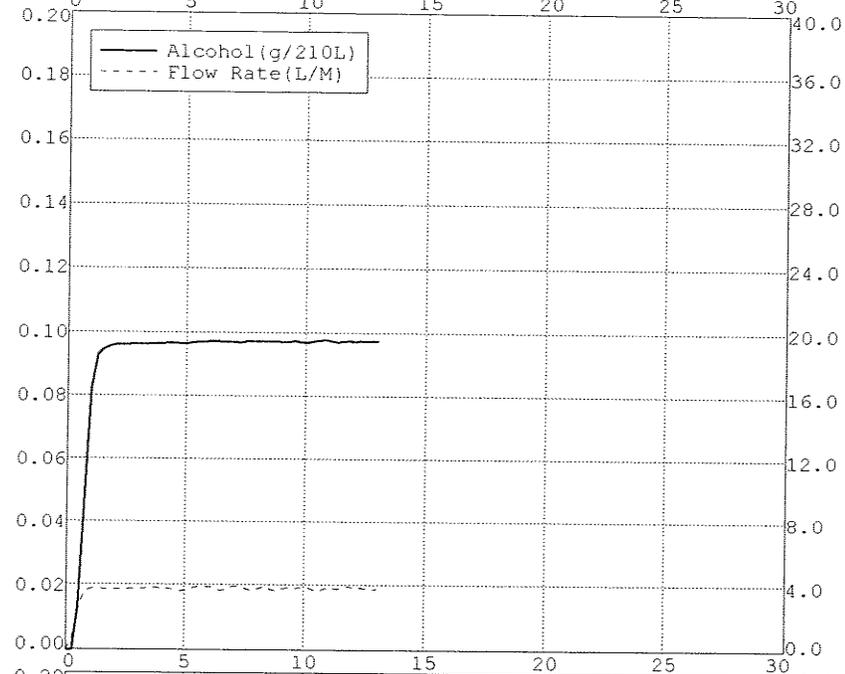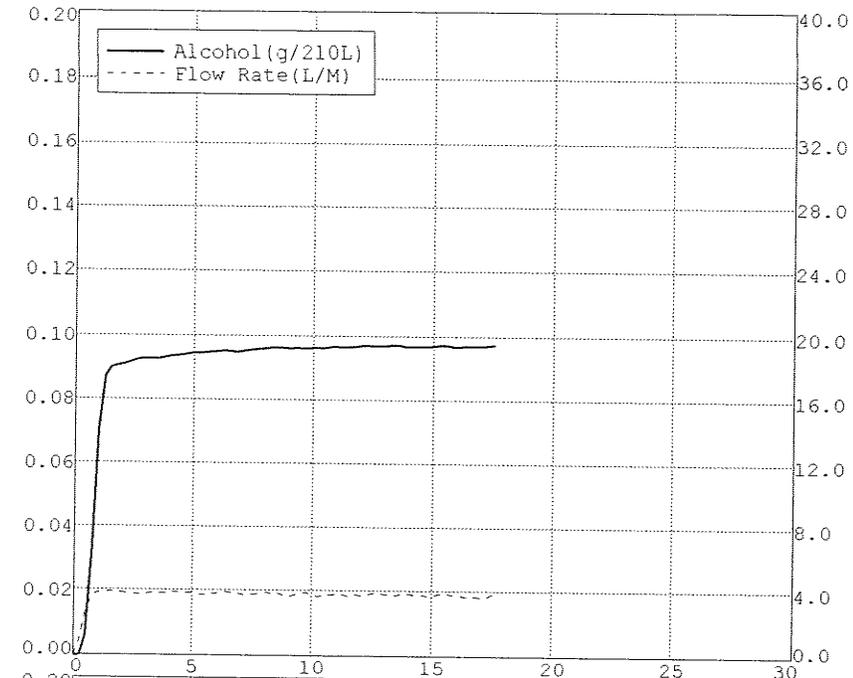

SUPERVISOR TEST

-----  
WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208  
-----

Date: 05/09/2018

OPERATOR NAME:  
J T COON  
Permit #: 36043  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18040

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:34
INTERNAL STANDARD	VERIFIED	00:34

Simulator Timed Out

*P.O. [Signature]* 341

SUPERVISOR TEST

-----  
WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208  
-----

Date: 05/09/2018

OPERATOR NAME:  
J T COON  
Permit #: 36043  
Operator Agency/Dept: WARREN CO SHERIFF'S  
OFFICE  
Reference Standard #: 18040

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:27
INTERNAL STANDARD	VERIFIED	00:27

Simulator Timed Out

*P.O. [Signature]* 3411

SUPERVISOR TEST

-----  
WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208  
-----

Date: 05/08/2018

OPERATOR NAME:  
J T COON  
Permit #: 36043  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18040

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:24
INTERNAL STANDARD	VERIFIED	21:24

Simulator Timed Out

*P. J. R. 341*