

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 05/15/2018

OPERATOR NAME:
TYLER J MORSE
Permit #: 41959
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18040

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:25
INTERNAL STANDARD	VERIFIED	13:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:26
BLANK TEST	0.00	13:27
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	13:27
BLANK TEST	0.00	13:28
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:29
BLANK TEST	0.00	13:30

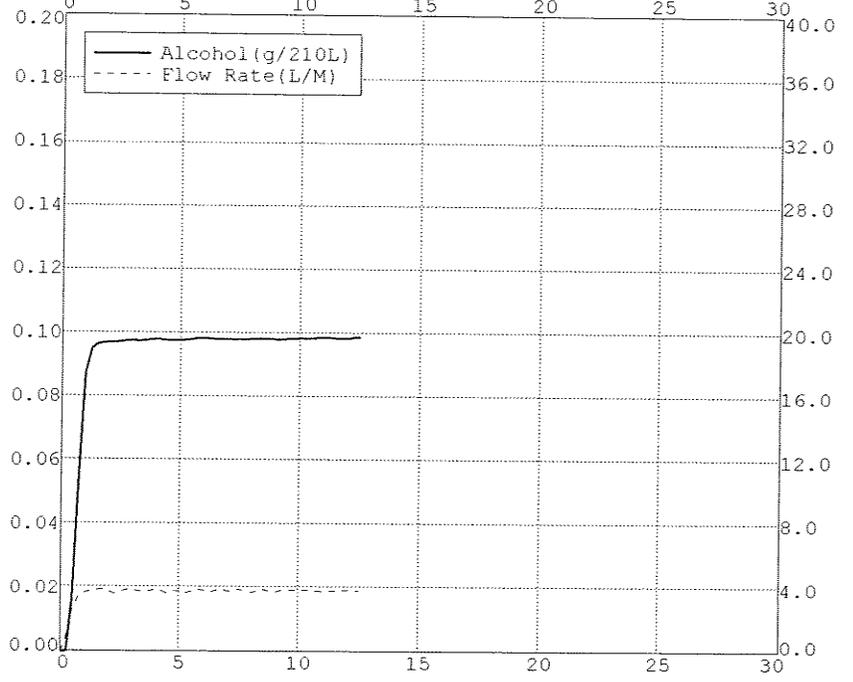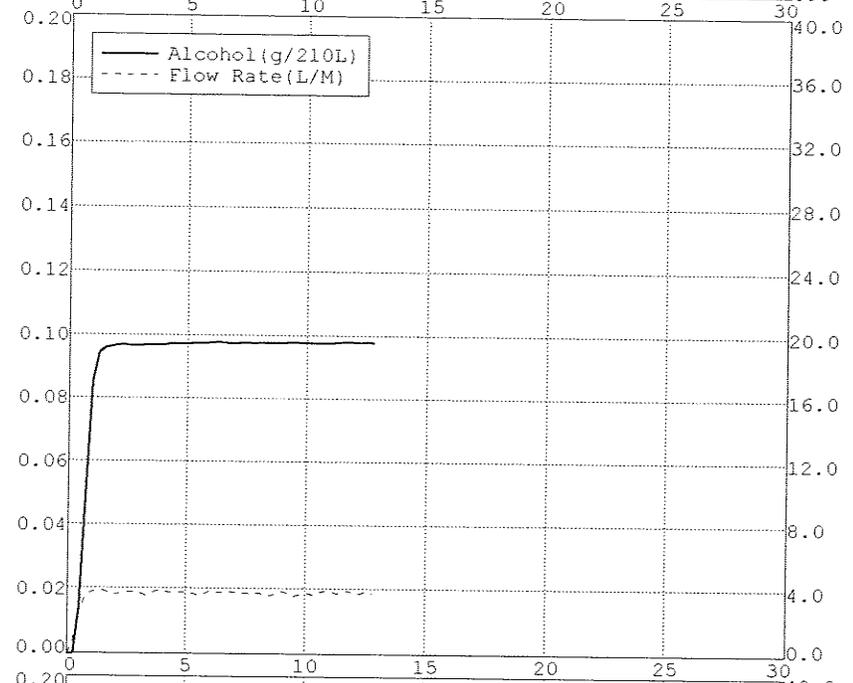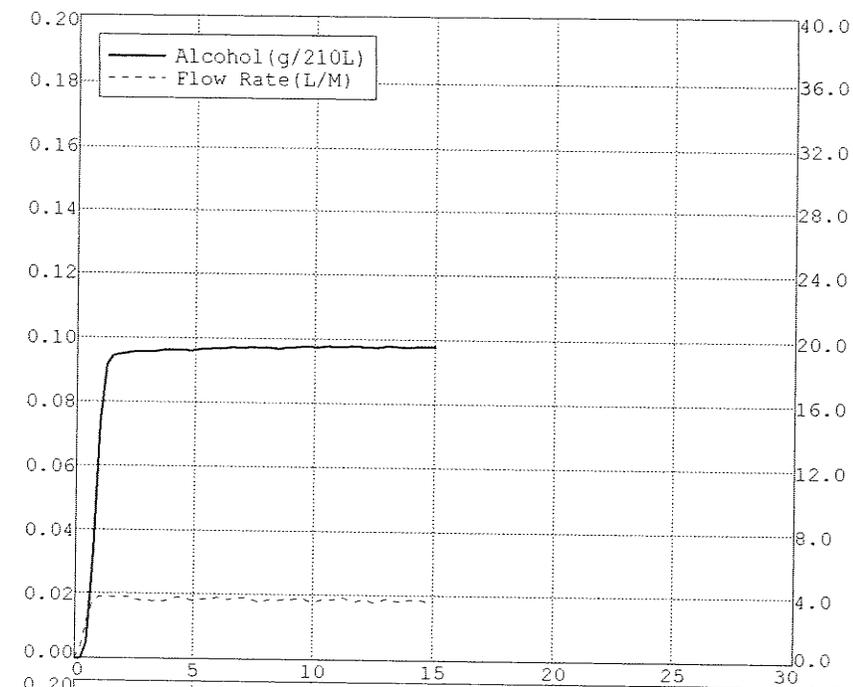

Pod #417