

SUPERVISOR TEST




 WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208

Date: 05/22/2018

OPERATOR NAME:
 J T COON
 Permit #: 36043
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 18040

Nominal = 0.10 g/210L

BLANK TEST	0.00	20:28
INTERNAL STANDARD	VERIFIED	20:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	20:28
BLANK TEST	0.00	20:29
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	20:29
BLANK TEST	0.00	20:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	20:31
BLANK TEST	0.00	20:32

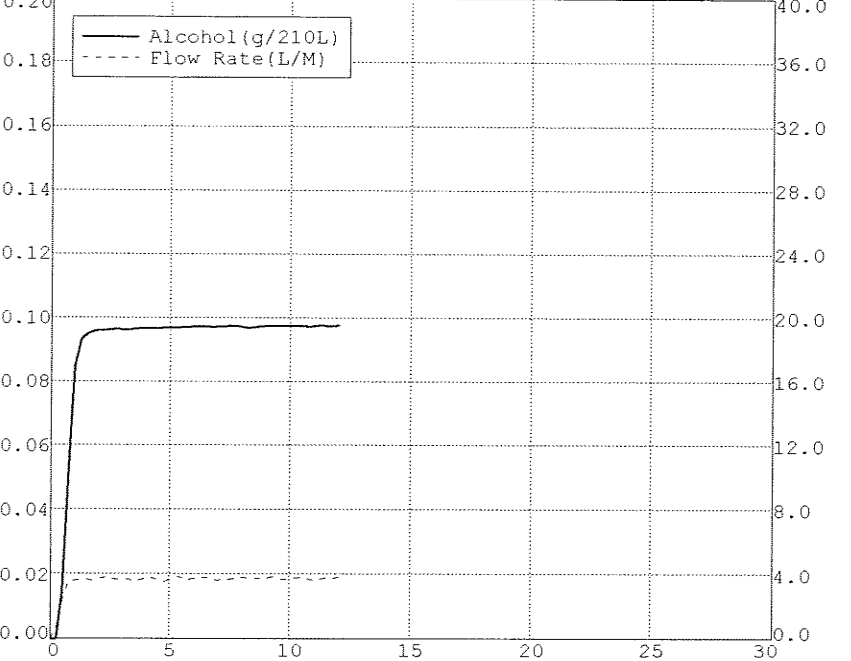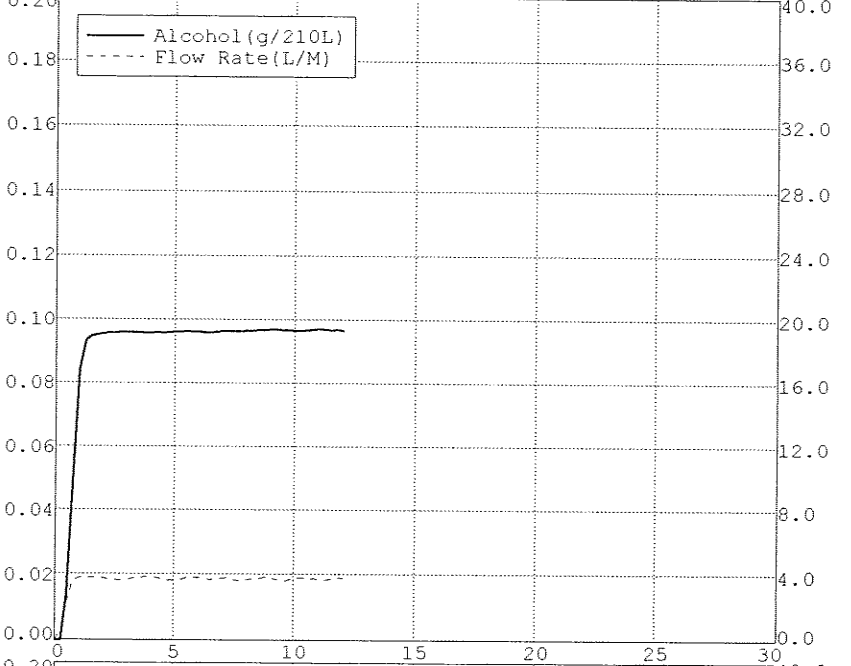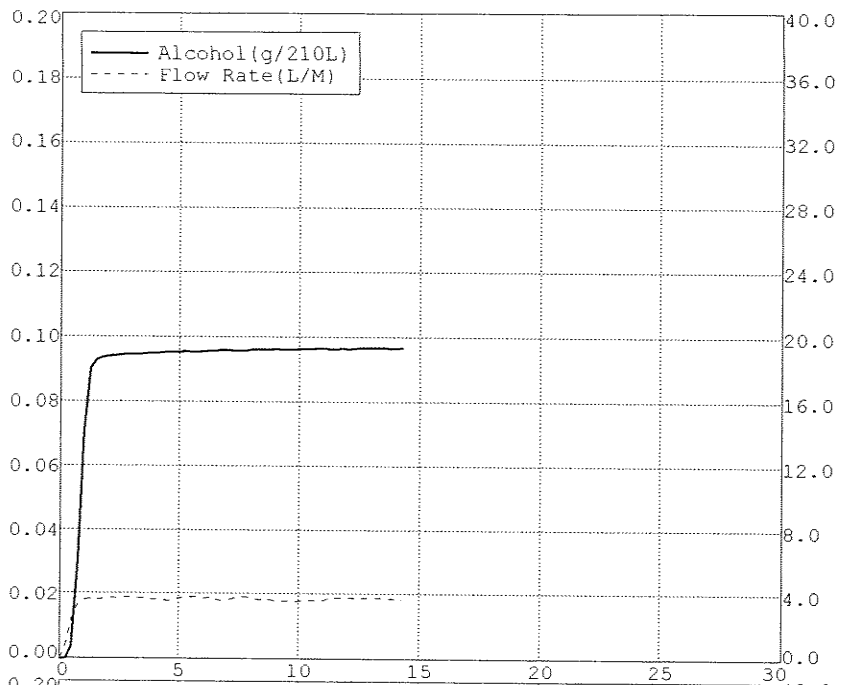

P. O. J. 341