

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 05/29/2018

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18040

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:31
INTERNAL STANDARD	VERIFIED	01:31
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:32
BLANK TEST	0.00	01:33
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.09	01:33
BLANK TEST	0.00	01:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	01:34
BLANK TEST	0.00	01:35

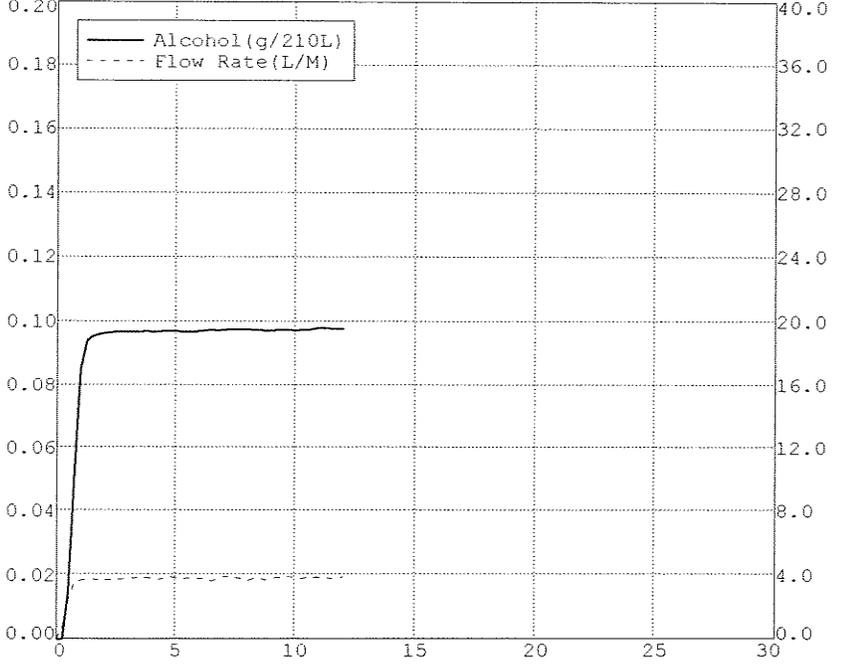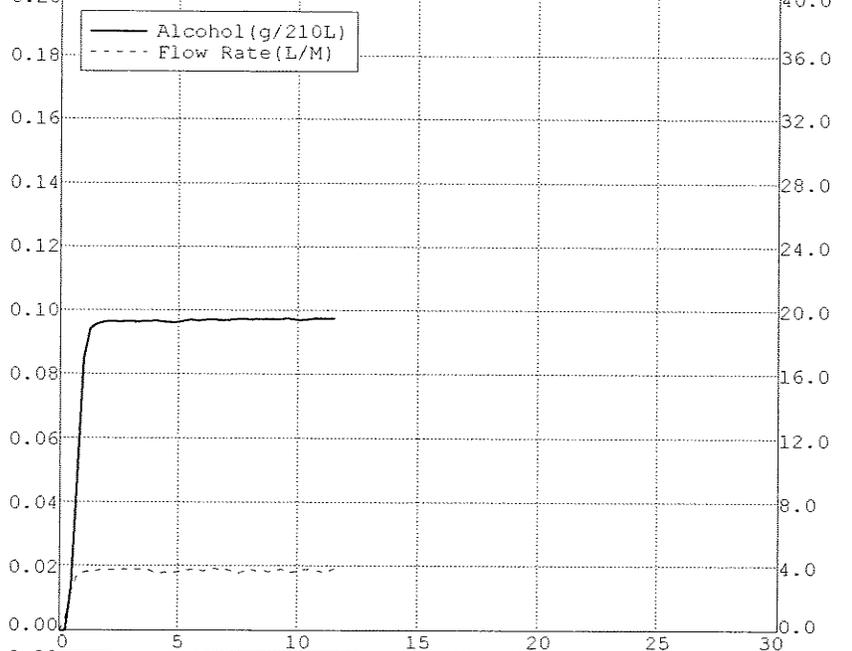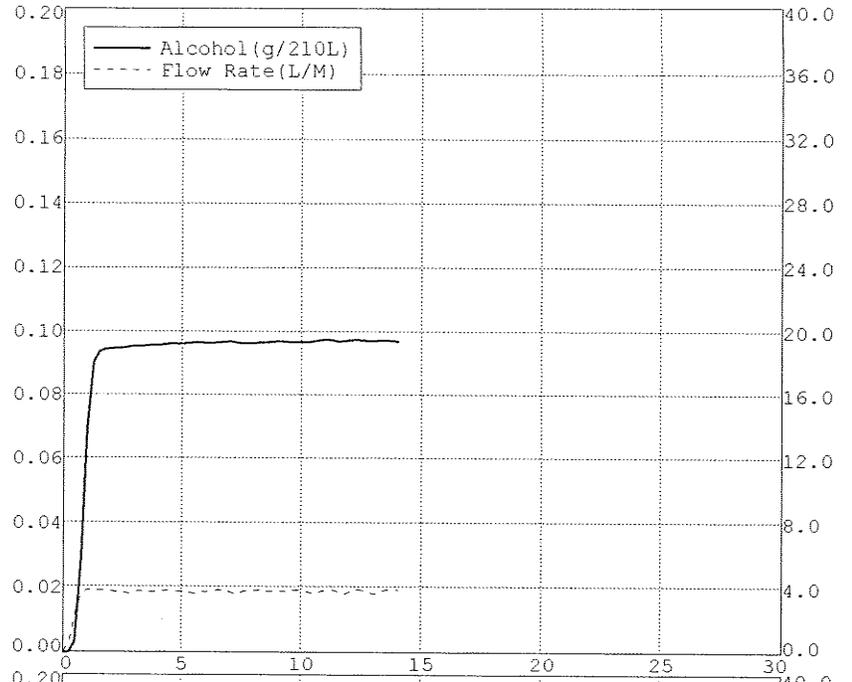

*Charles B Geisler* #201