

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 06/02/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18100

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:40
INTERNAL STANDARD	VERIFIED	02:40
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:41
BLANK TEST	0.00	02:42
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	02:42
BLANK TEST	0.00	02:43
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:43
BLANK TEST	0.00	02:44

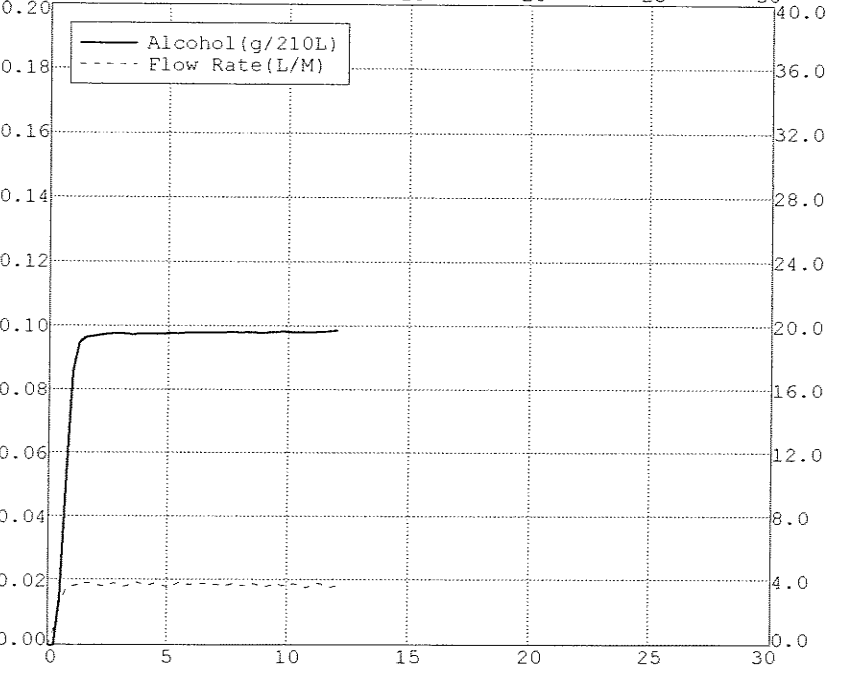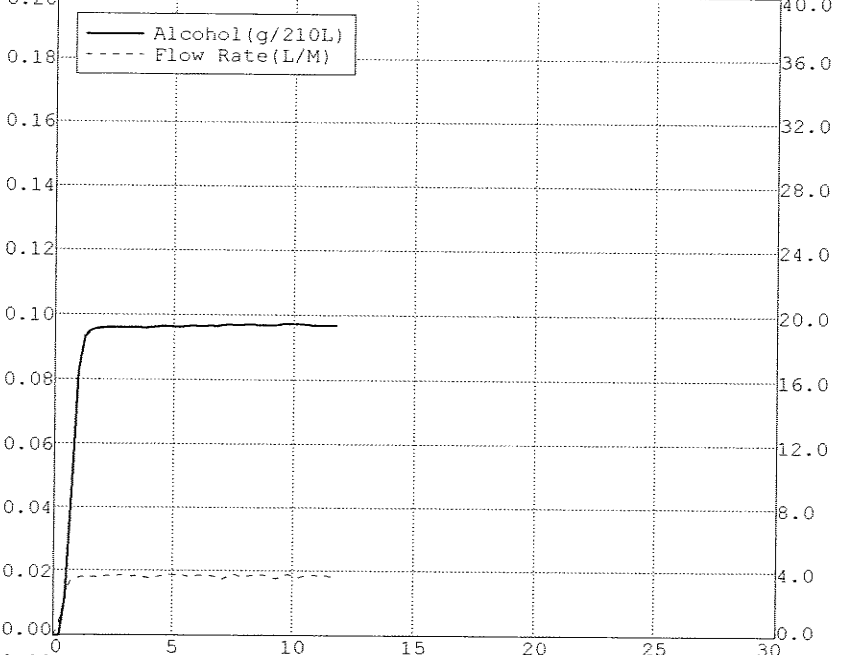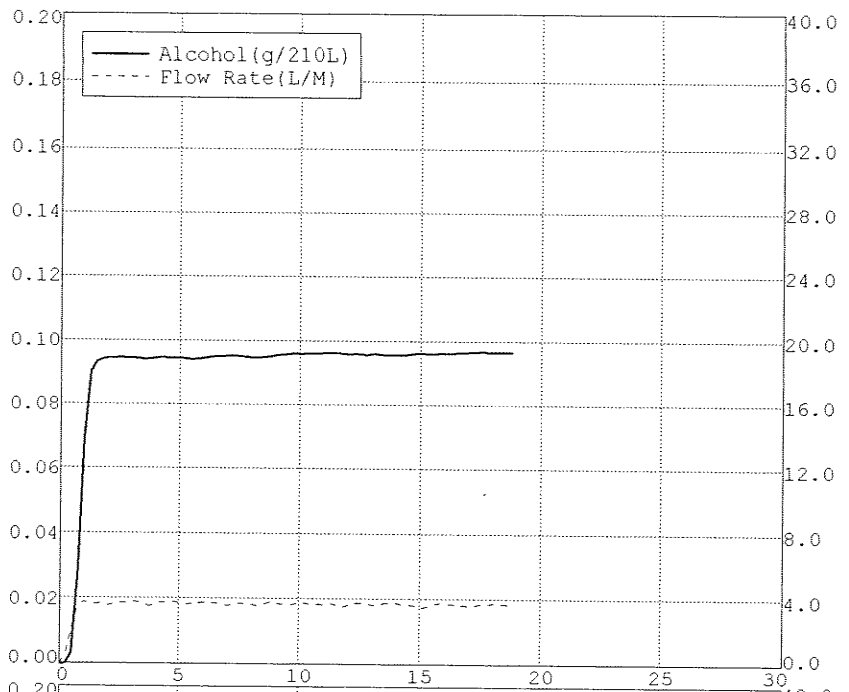

Handwritten signatures and initials:
J. [unclear] [unclear] [unclear] [unclear]