

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 06/09/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18100

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:49
INTERNAL STANDARD	VERIFIED	21:50
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:50
BLANK TEST	0.00	21:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:51
BLANK TEST	0.00	21:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	21:52
BLANK TEST	0.00	21:53

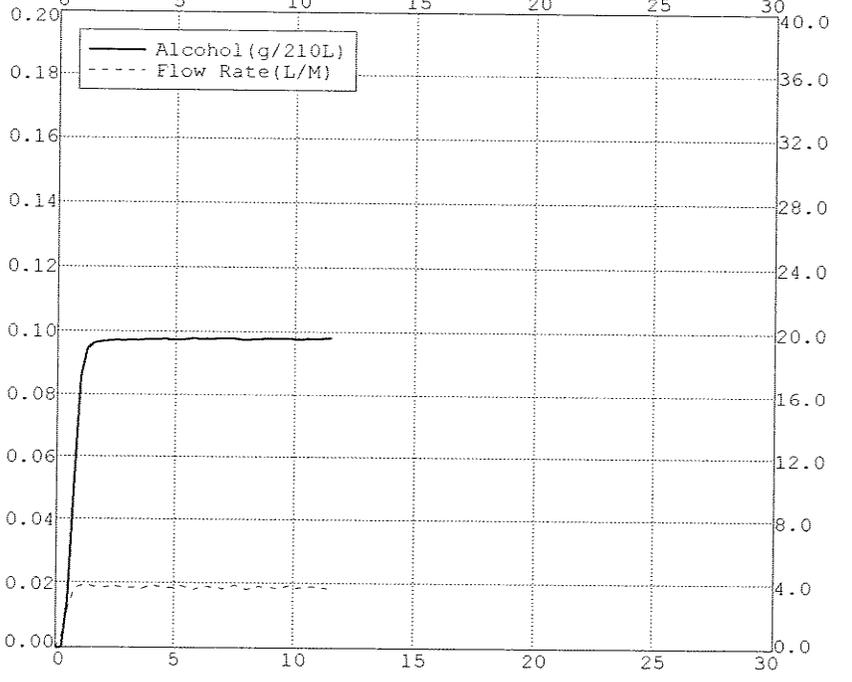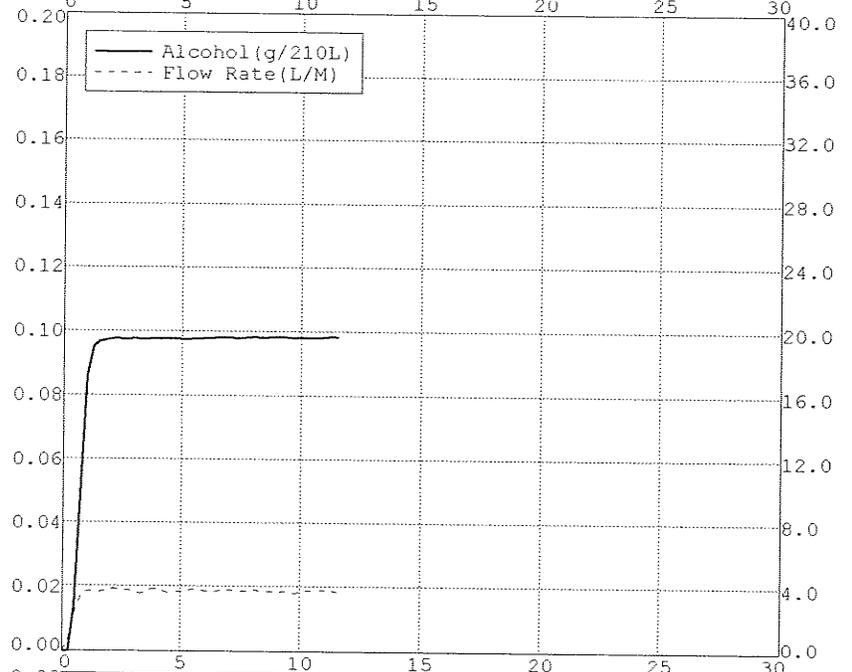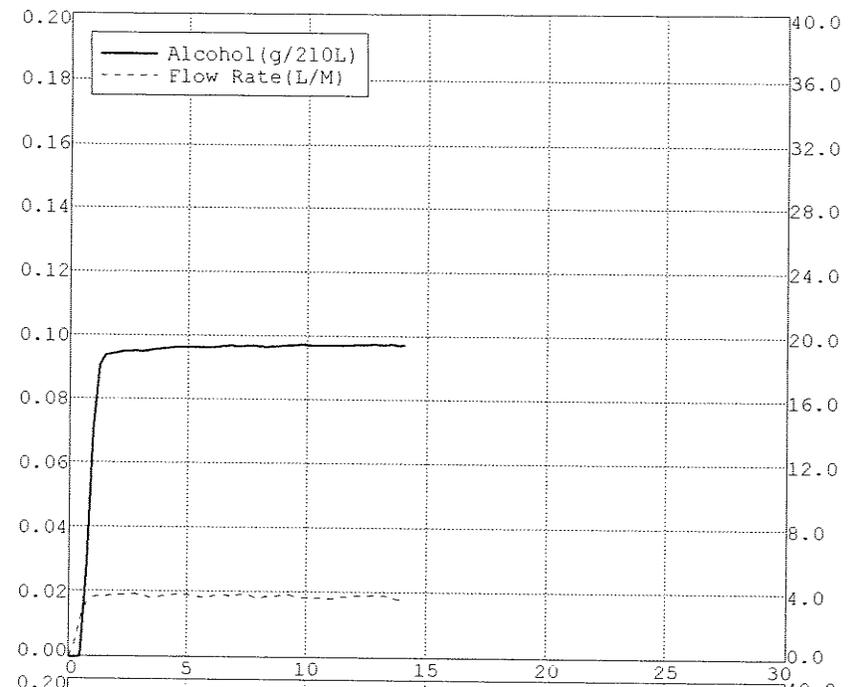

Charles B. Geisler