

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 06/16/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18100

Nominal = 0.10 g/210L

BLANK TEST	0.00	01:58
INTERNAL STANDARD	VERIFIED	01:58
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	01:58
BLANK TEST	0.00	01:59
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	02:00
BLANK TEST	0.00	02:00
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:01
BLANK TEST	0.00	02:02

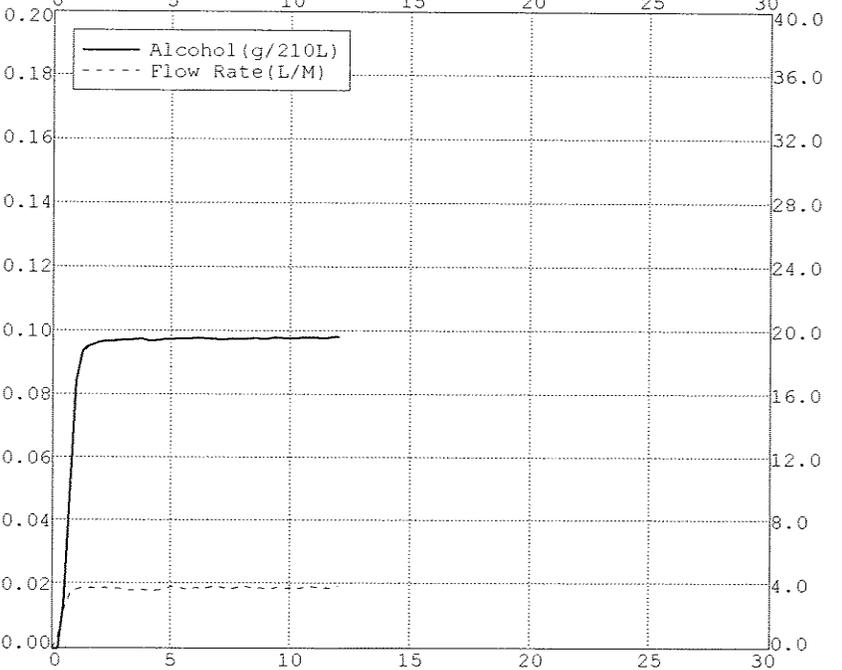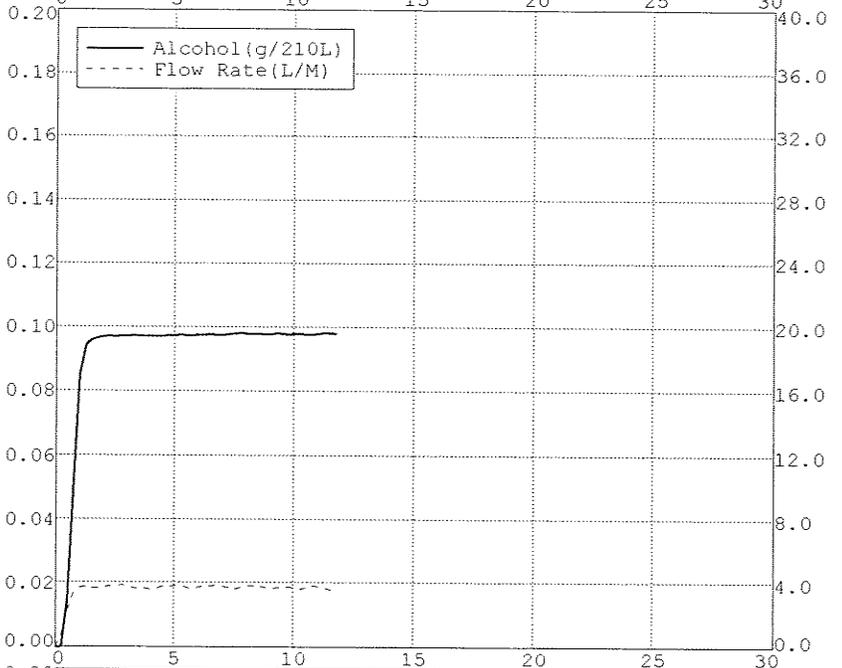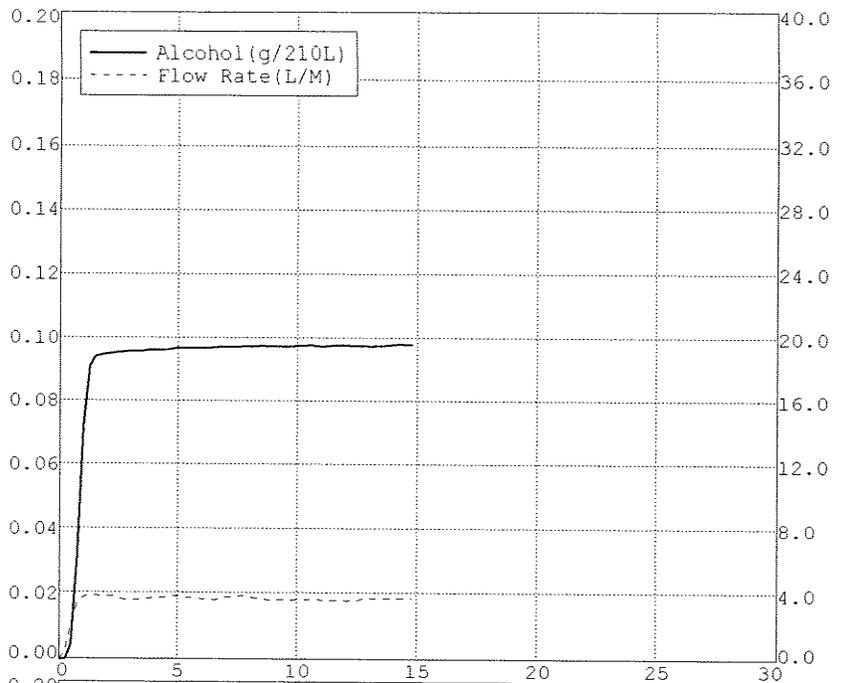

Charles B. Geisler