

SUPERVISOR TEST


WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 06/29/2018

OPERATOR NAME:
RYAN C SCHROECK
Permit #: 41316
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18100

Nominal = 0.10 g/210L

BLANK TEST	0.00	08:41
INTERNAL STANDARD	VERIFIED	08:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	08:42
BLANK TEST	0.00	08:43
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	08:43
BLANK TEST	0.00	08:44
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	08:45
BLANK TEST	0.00	08:45

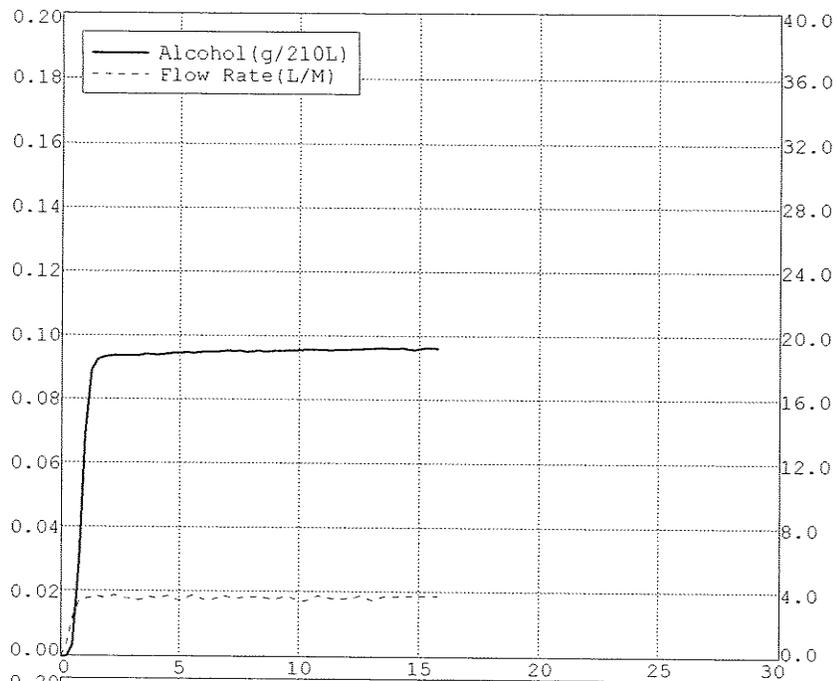

100 *RS* 724