

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 07/15/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18100

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:43
INTERNAL STANDARD	VERIFIED	04:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	04:44
BLANK TEST	0.00	04:45
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.09	04:45
BLANK TEST	0.00	04:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	04:46
BLANK TEST	0.00	04:47

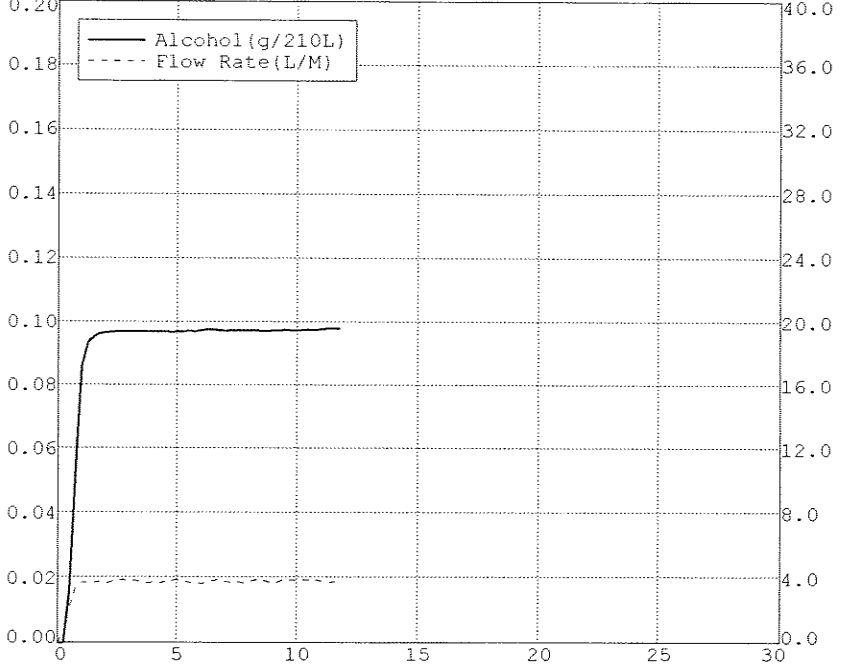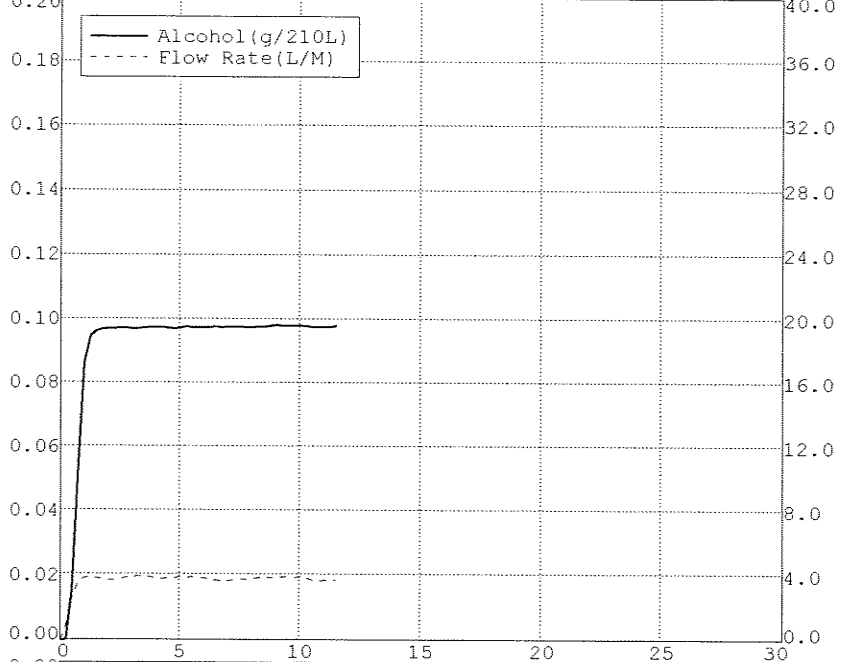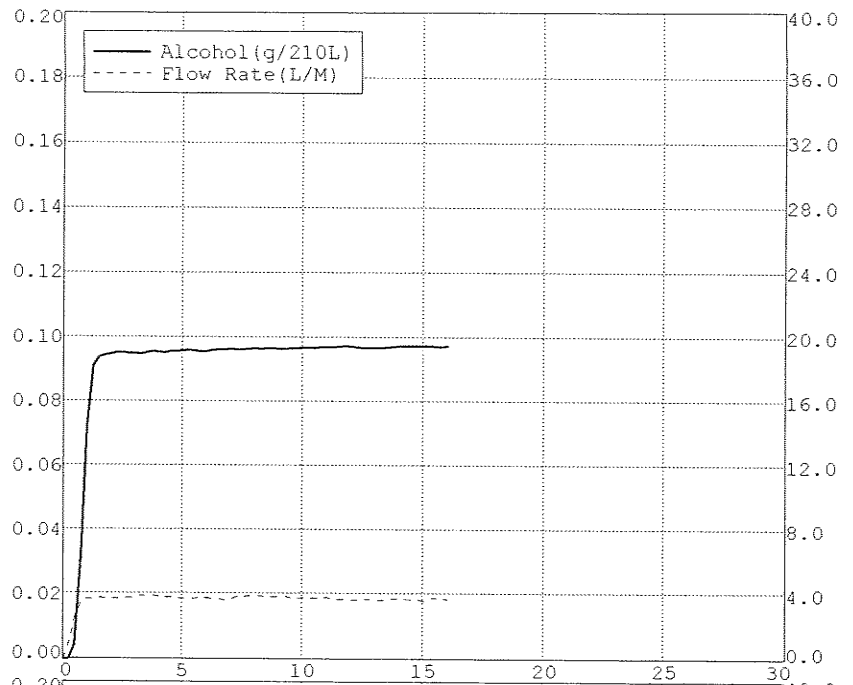

Charles B. Geisler #248