

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 07/29/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18100

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:30
INTERNAL STANDARD	VERIFIED	02:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	02:31
BLANK TEST	0.00	02:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	02:32
BLANK TEST	0.00	02:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	02:33
BLANK TEST	0.00	02:34

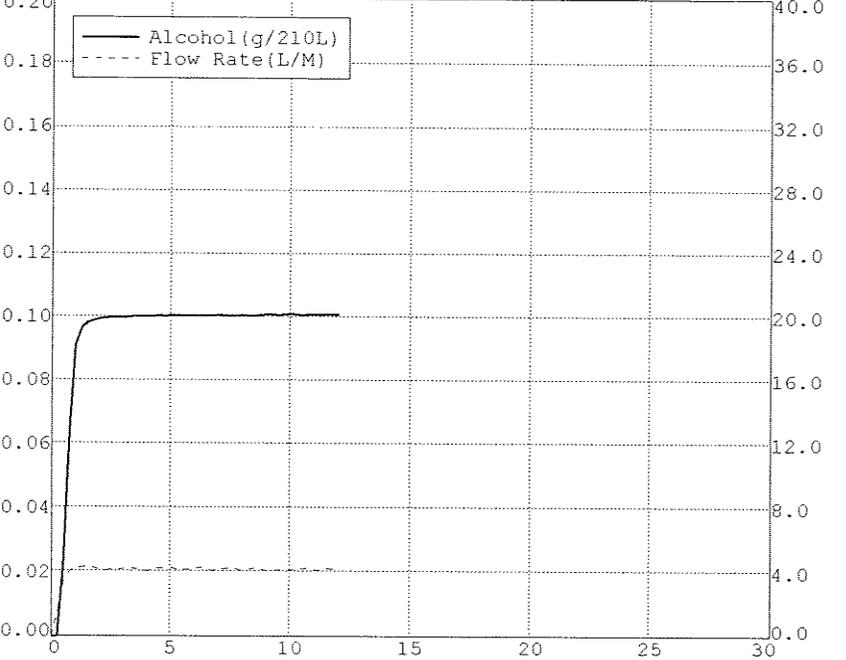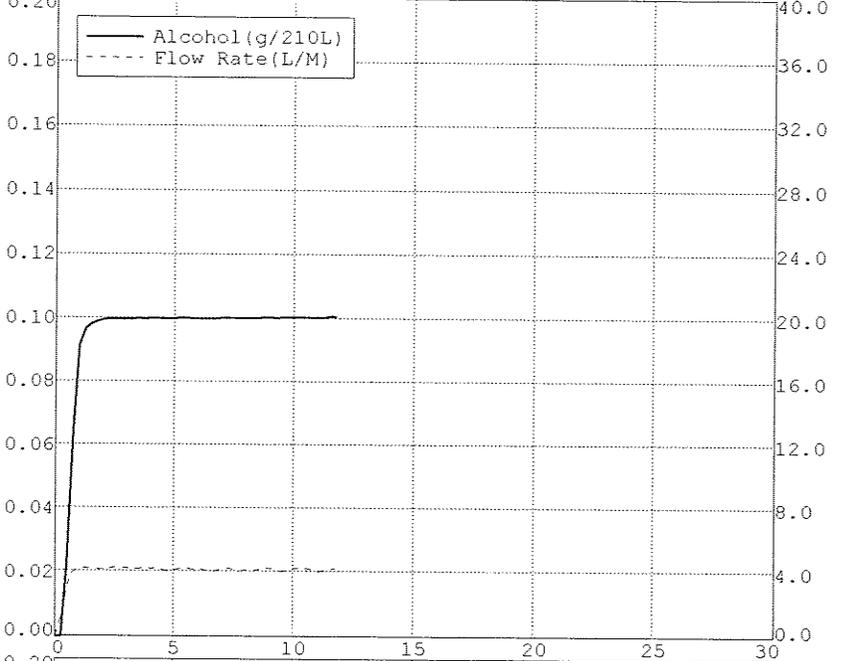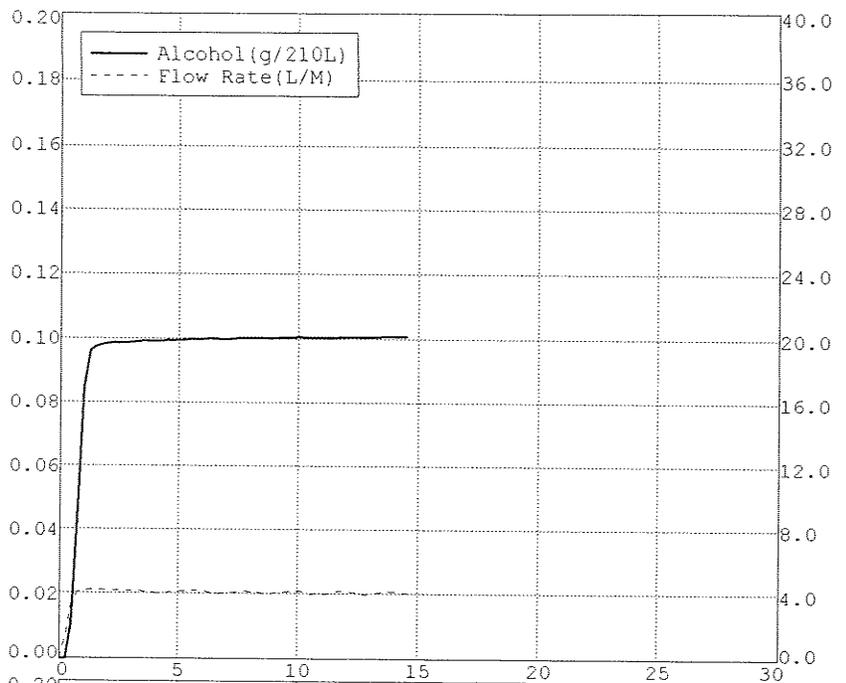

Charles B Geisler #241