

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 08/03/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18170

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:26
INTERNAL STANDARD	VERIFIED	04:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	04:27
BLANK TEST	0.00	04:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	04:28
BLANK TEST	0.00	04:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	04:29
BLANK TEST	0.00	04:30

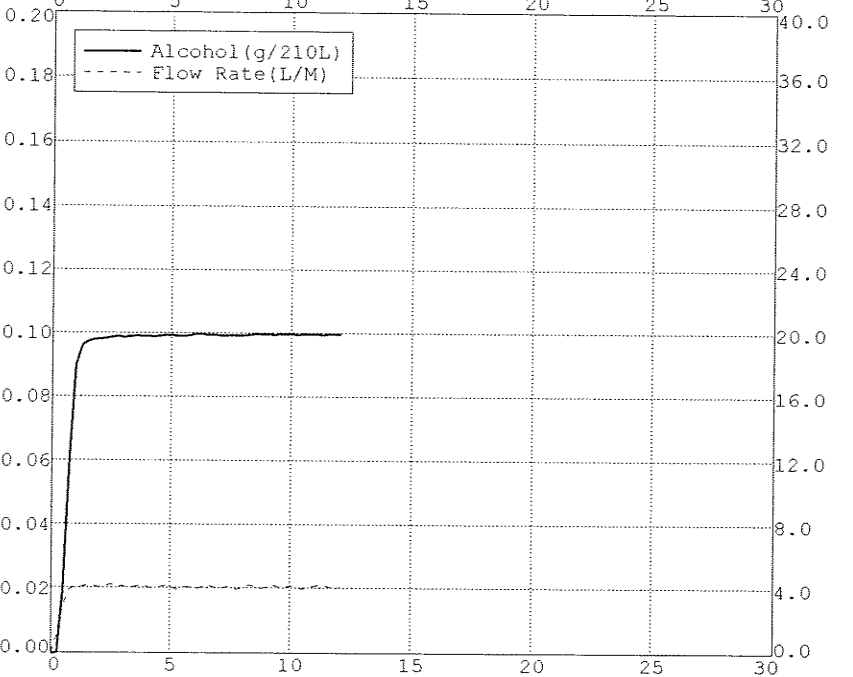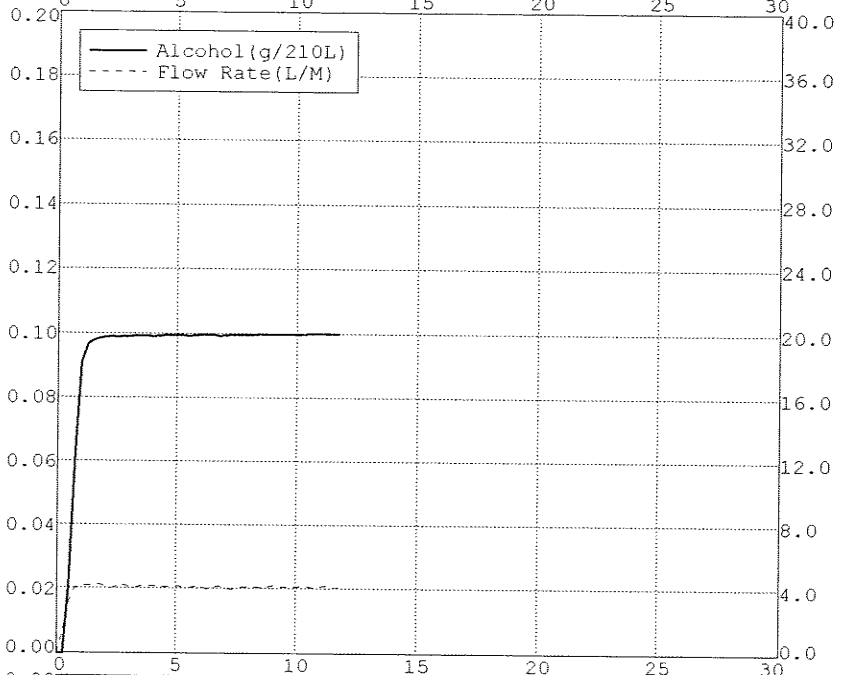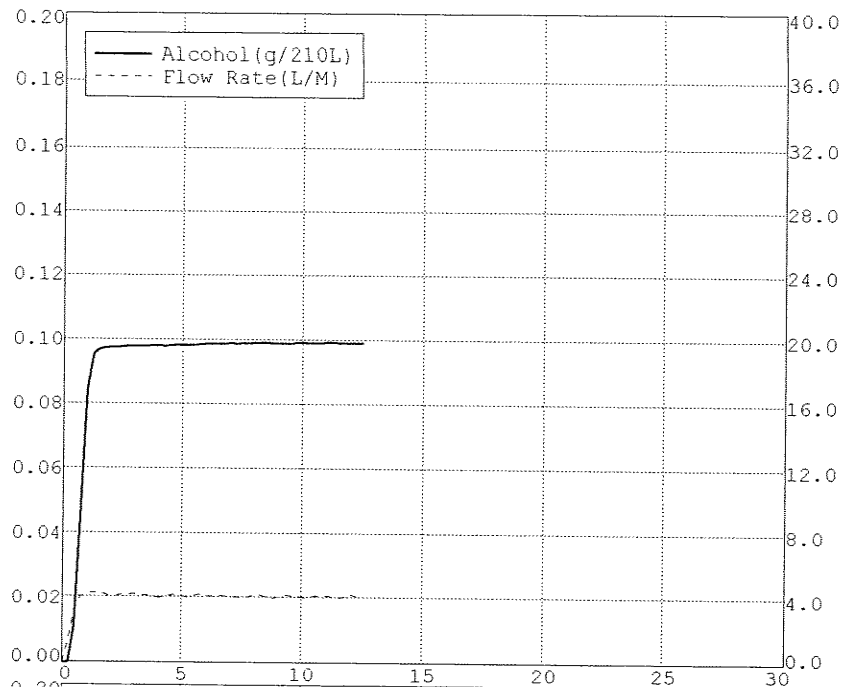

Charles B. Geisler