

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 08/08/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18170

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:29
INTERNAL STANDARD	VERIFIED	00:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	00:30
BLANK TEST	0.00	00:31
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	00:31
BLANK TEST	0.00	00:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	00:33
BLANK TEST	0.00	00:34

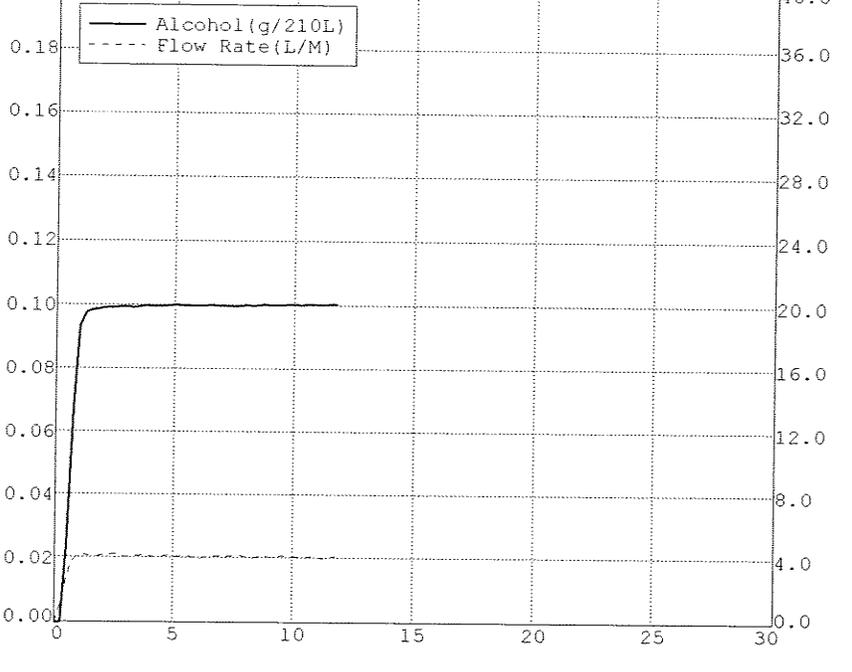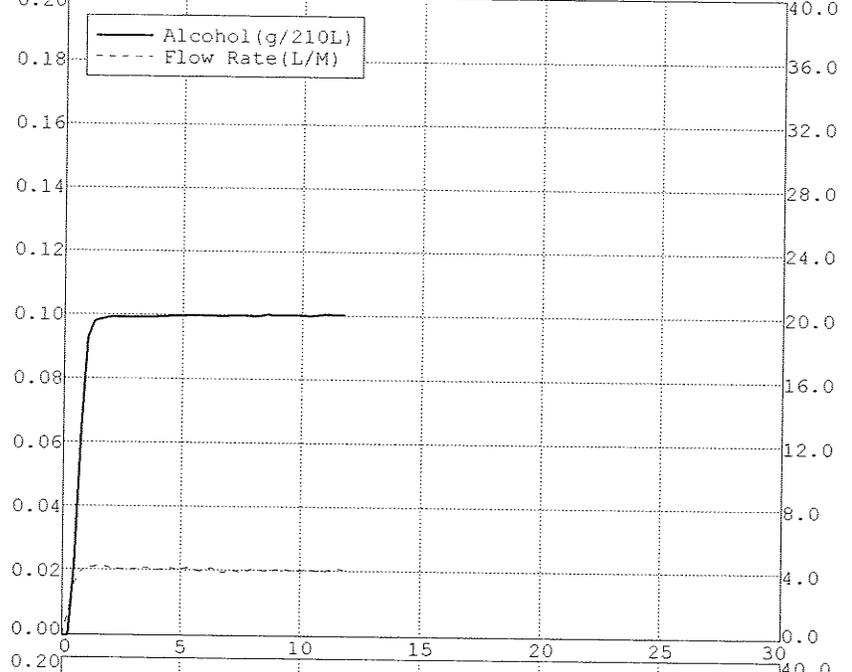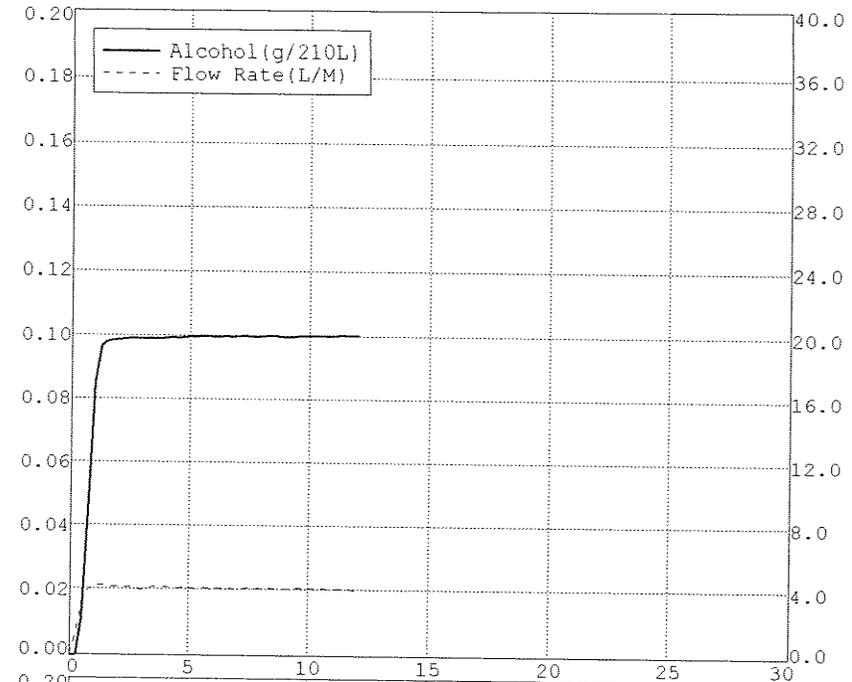

Charles B. Geisler #211