

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 09/10/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18170

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:16
INTERNAL STANDARD	VERIFIED	02:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	02:16
BLANK TEST	0.00	02:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	02:17
BLANK TEST	0.00	02:18
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	02:19
BLANK TEST	0.00	02:20

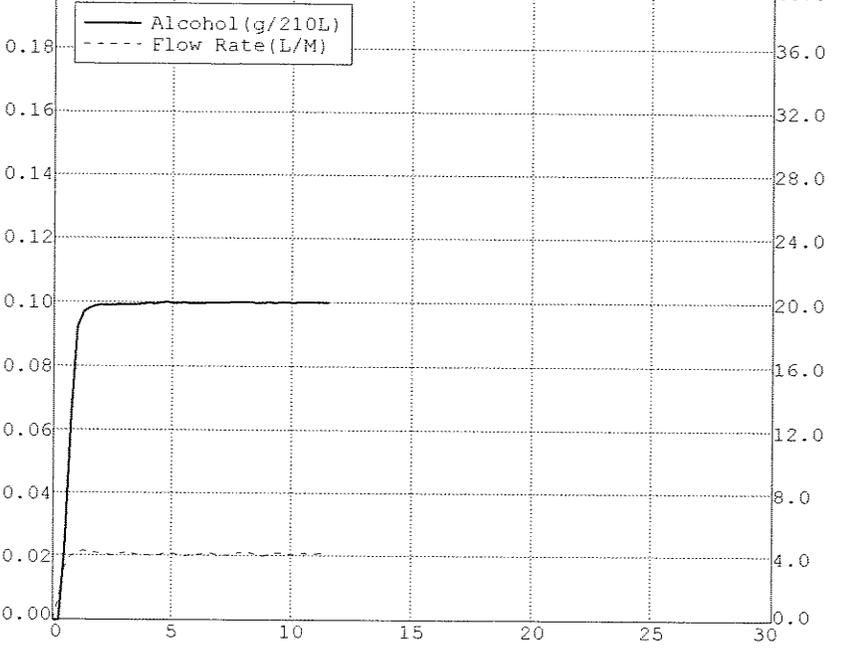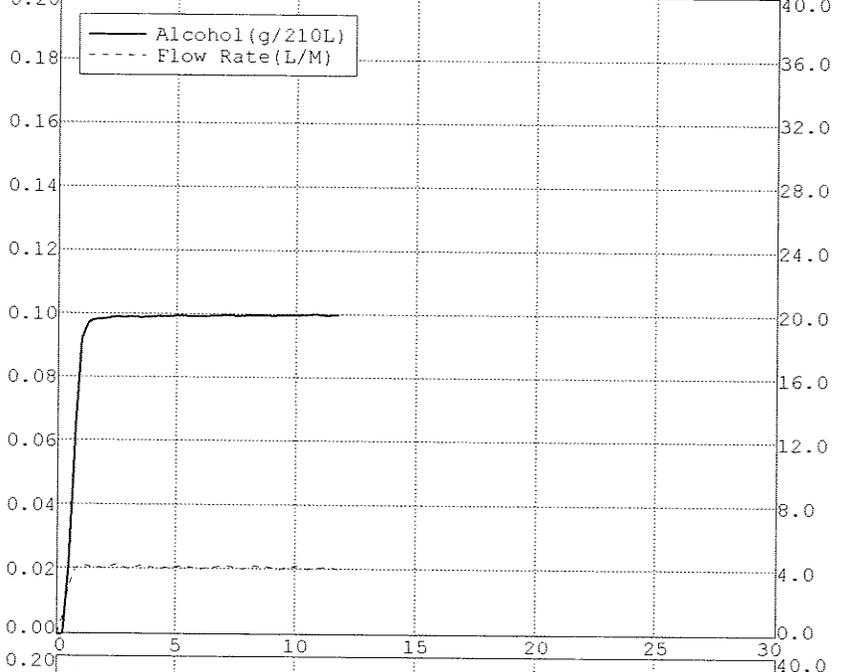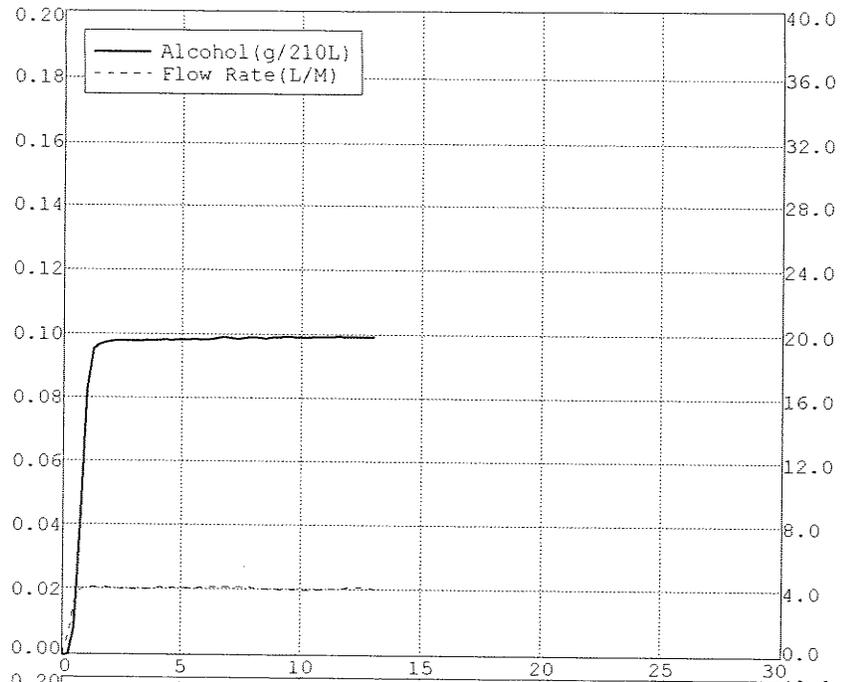

Charles B. Geisler #2