

SUPERVISOR TEST



WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 09/19/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18170

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:51
INTERNAL STANDARD	VERIFIED	05:51
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:52
BLANK TEST	0.00	05:53
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:53
BLANK TEST	0.00	05:54
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	05:54
BLANK TEST	0.00	05:55

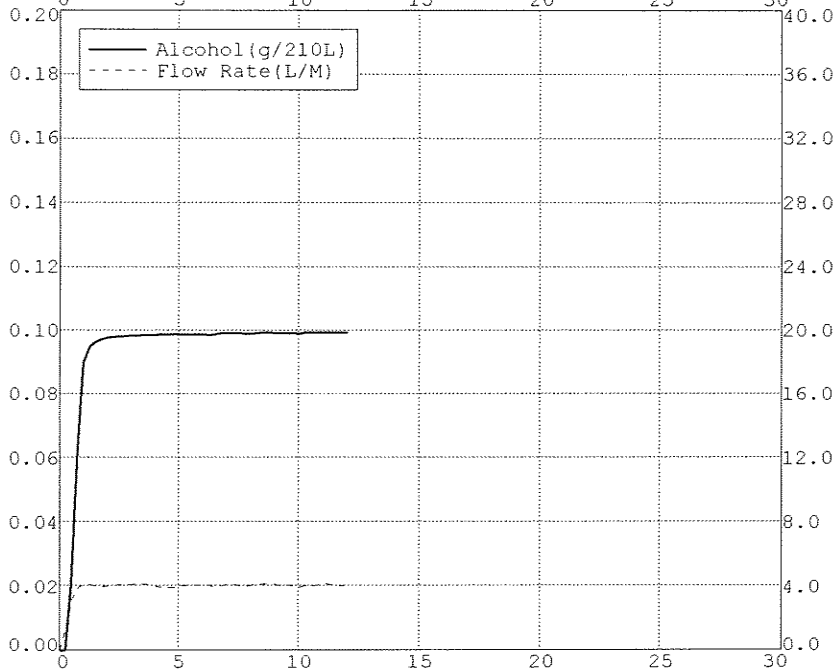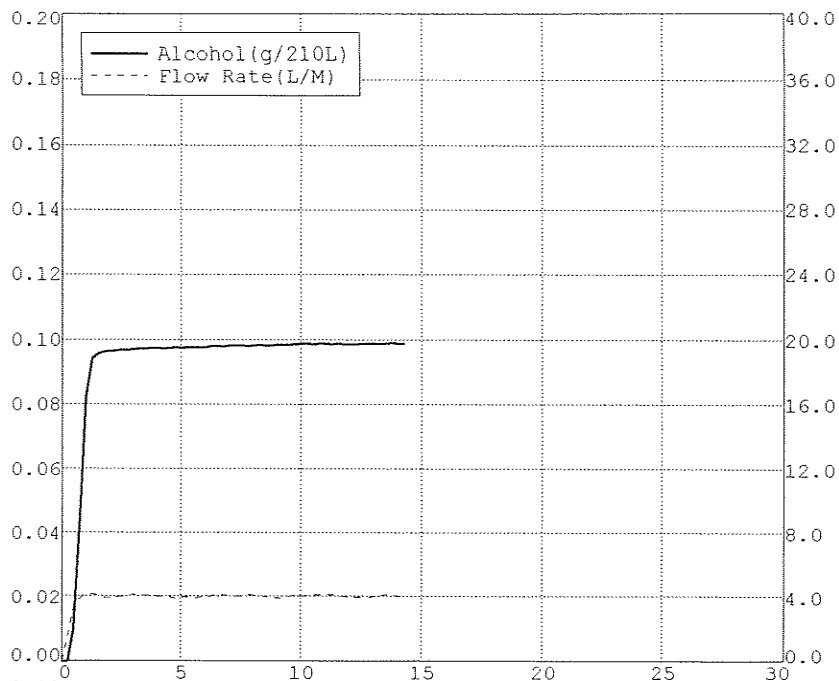

Charles B. Geisler #244