

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 10/02/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18230

Nominal = 0.10 g/210L

BLANK TEST	0.00	03:44
INTERNAL STANDARD	VERIFIED	03:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	03:45
BLANK TEST	0.00	03:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	03:46
BLANK TEST	0.00	03:47
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	03:48
BLANK TEST	0.00	03:49

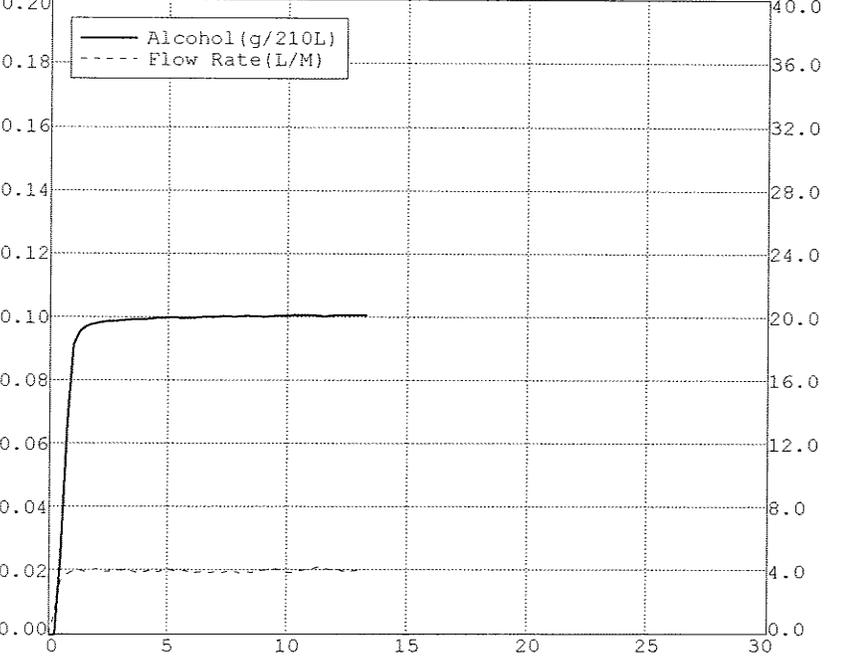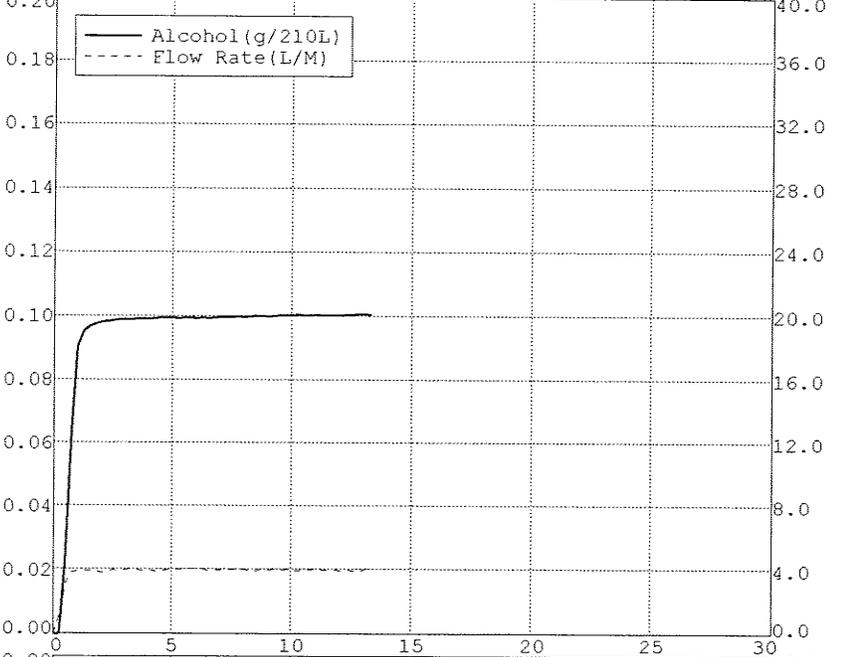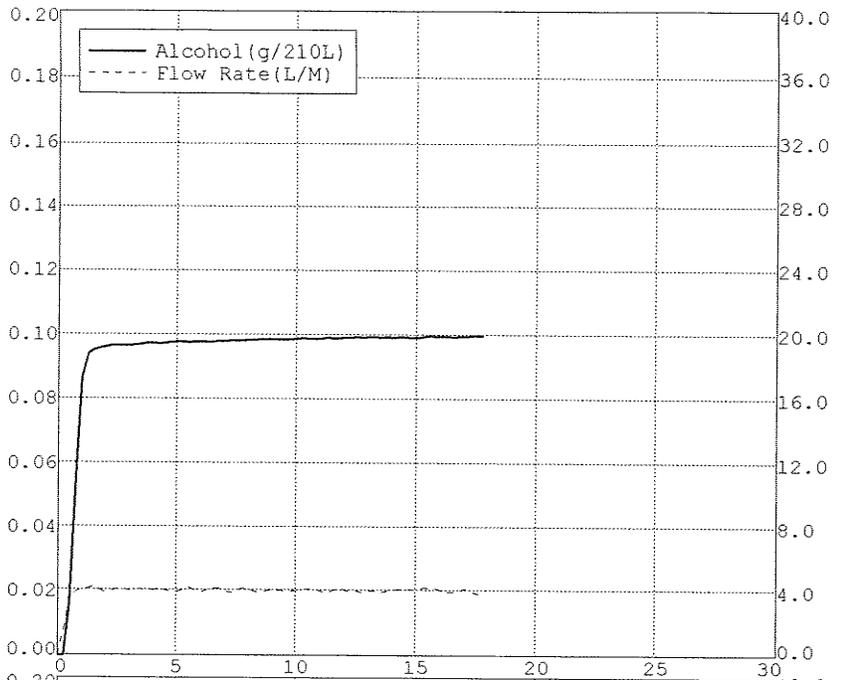

Charles B. Geisler