

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 11/08/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18230

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:57
INTERNAL STANDARD	VERIFIED	02:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	02:57
BLANK TEST	0.00	02:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	02:58
BLANK TEST	0.00	02:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	03:00
BLANK TEST	0.00	03:01

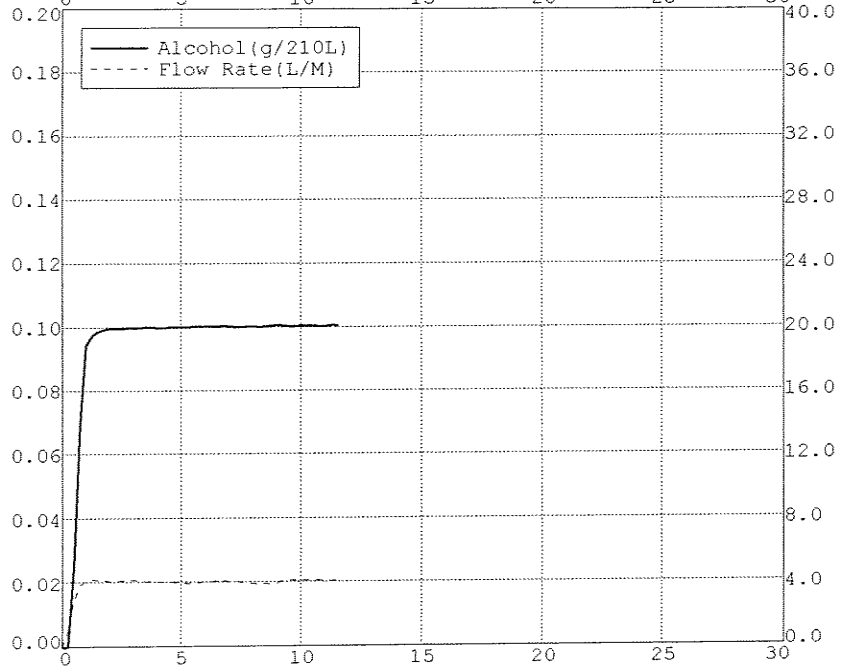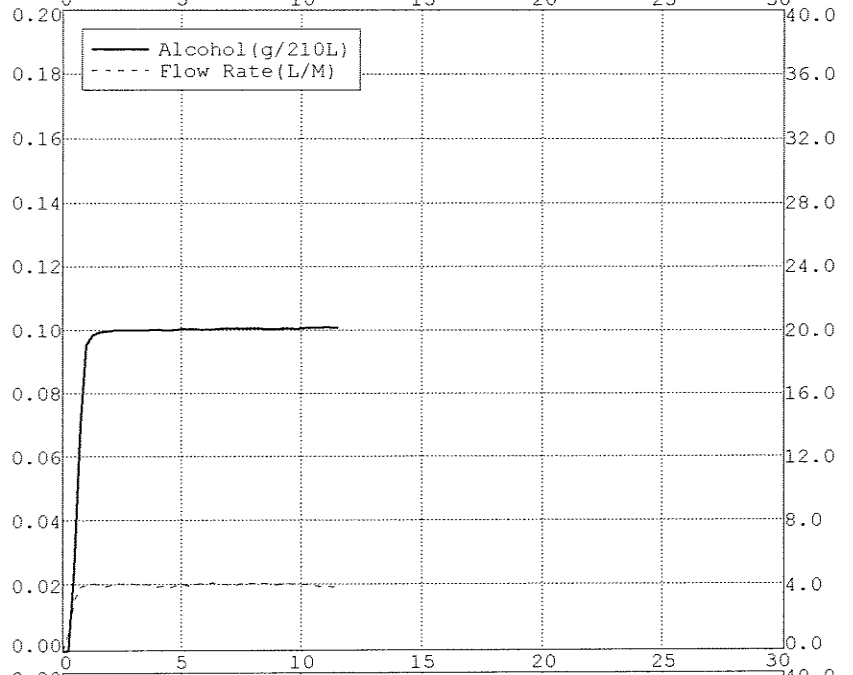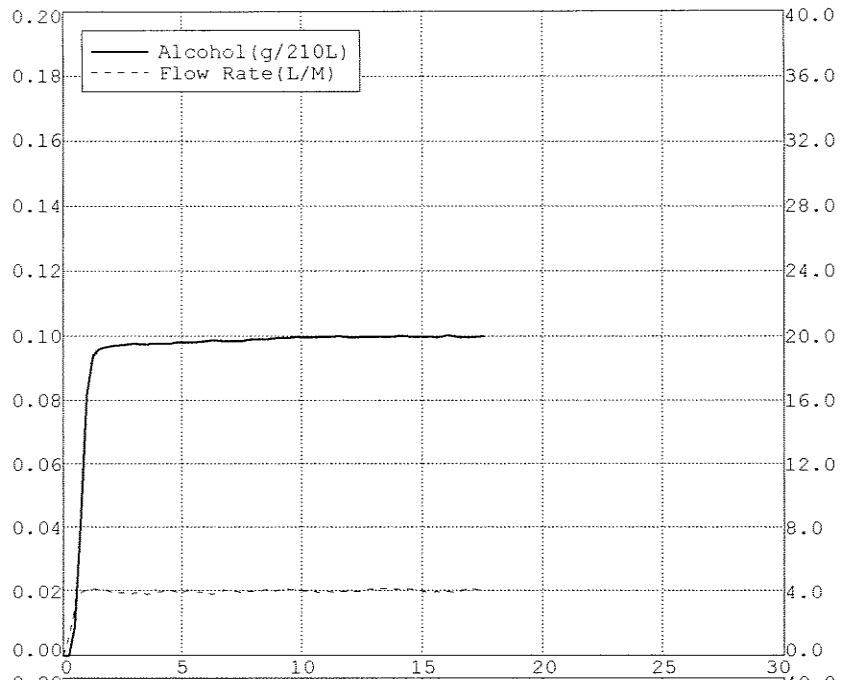

Charles B. Geisler #211