

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 11/14/2018

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 18230

Nominal = 0.10 g/210L

BLANK TEST	0.00	04:39
INTERNAL STANDARD	VERIFIED	04:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	04:39
BLANK TEST	0.00	04:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	04:40
BLANK TEST	0.00	04:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	04:42
BLANK TEST	0.00	04:43

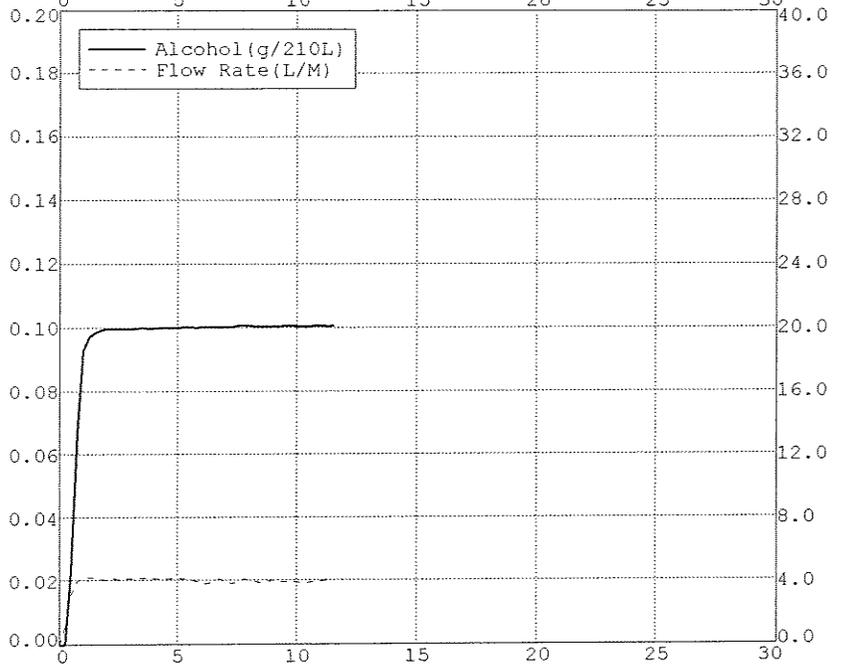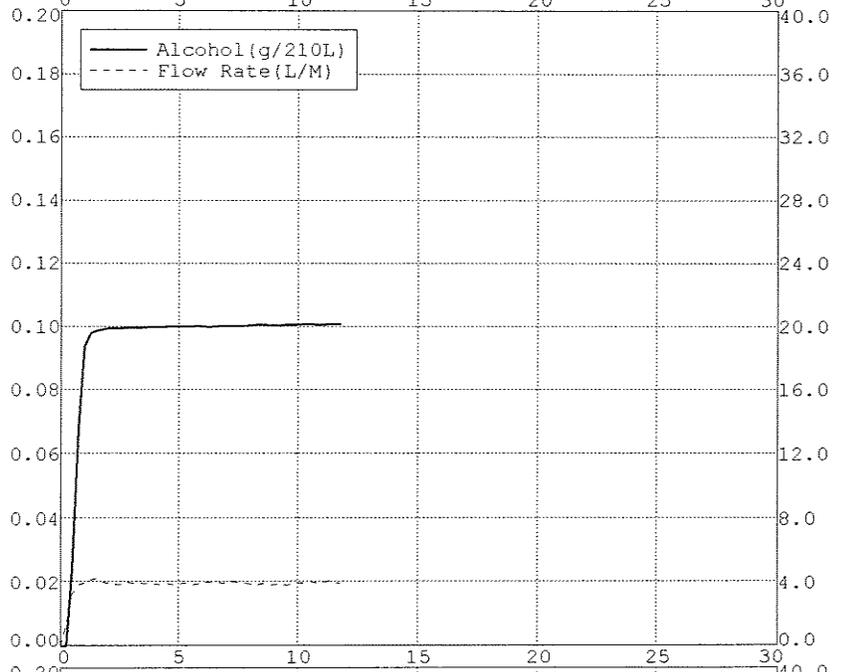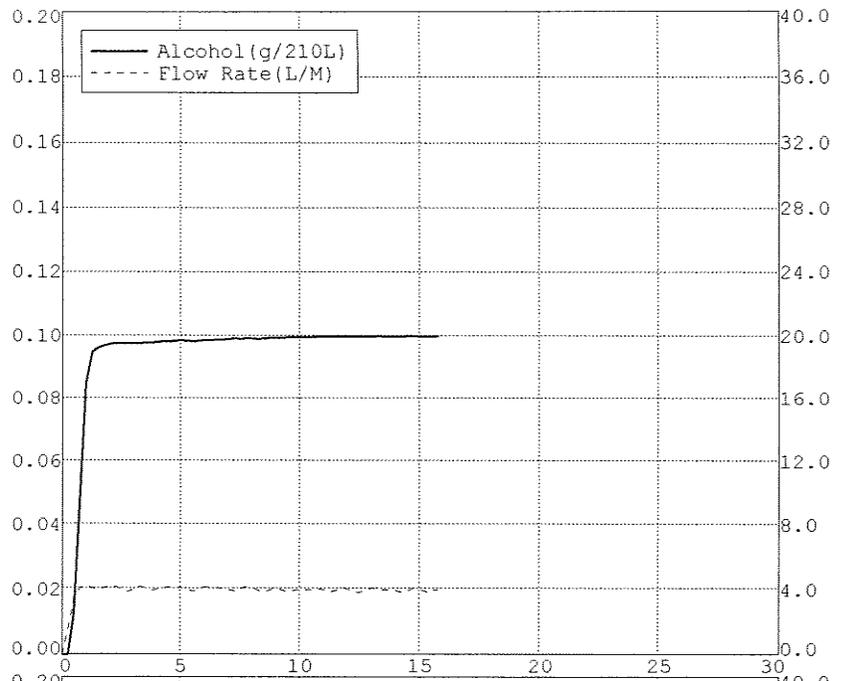

*[Handwritten signatures and initials]*