

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 11/27/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18230

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:08
INTERNAL STANDARD	VERIFIED	05:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	05:09
BLANK TEST	0.00	05:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	05:10
BLANK TEST	0.00	05:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	05:11
BLANK TEST	0.00	05:12

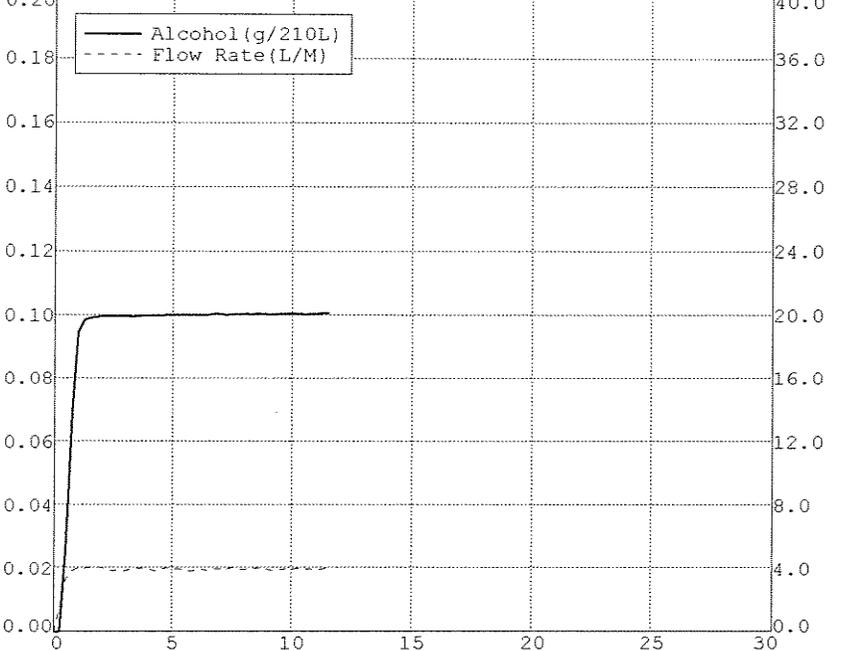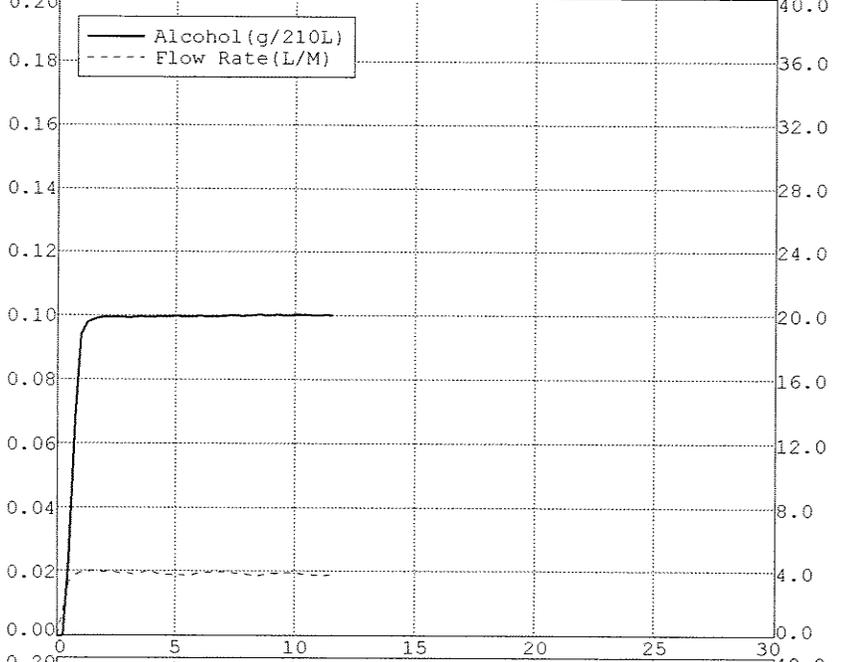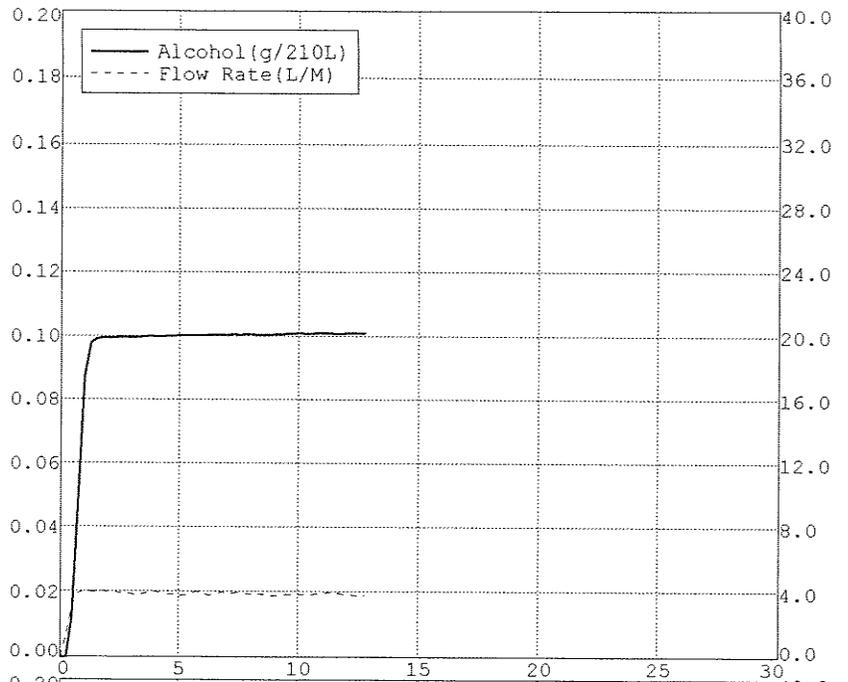

Charles B. Geisler #2011