

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 12/05/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	21:59
INTERNAL STANDARD	VERIFIED	21:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	21:59
BLANK TEST	0.00	22:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	22:00
BLANK TEST	0.00	22:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	22:02
BLANK TEST	0.00	22:03

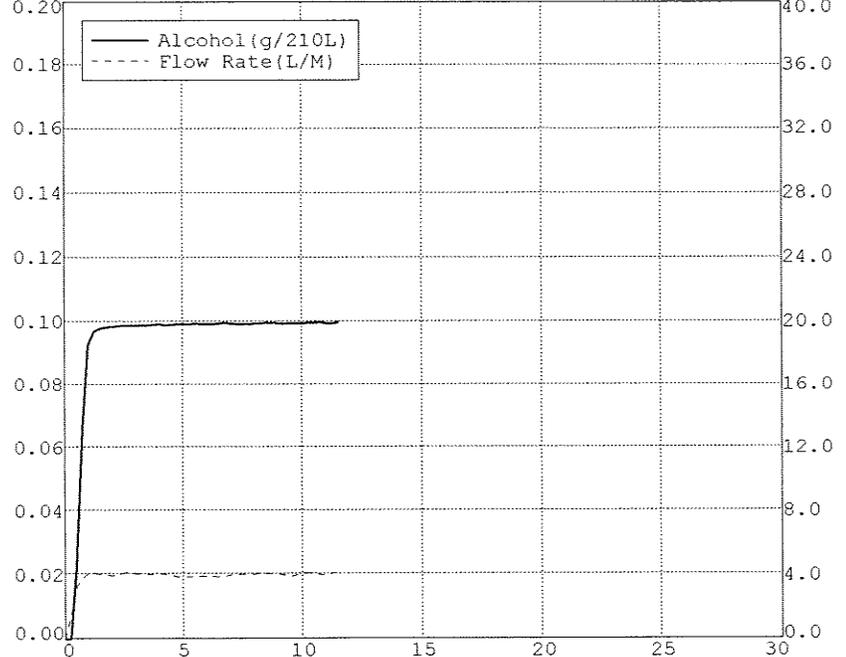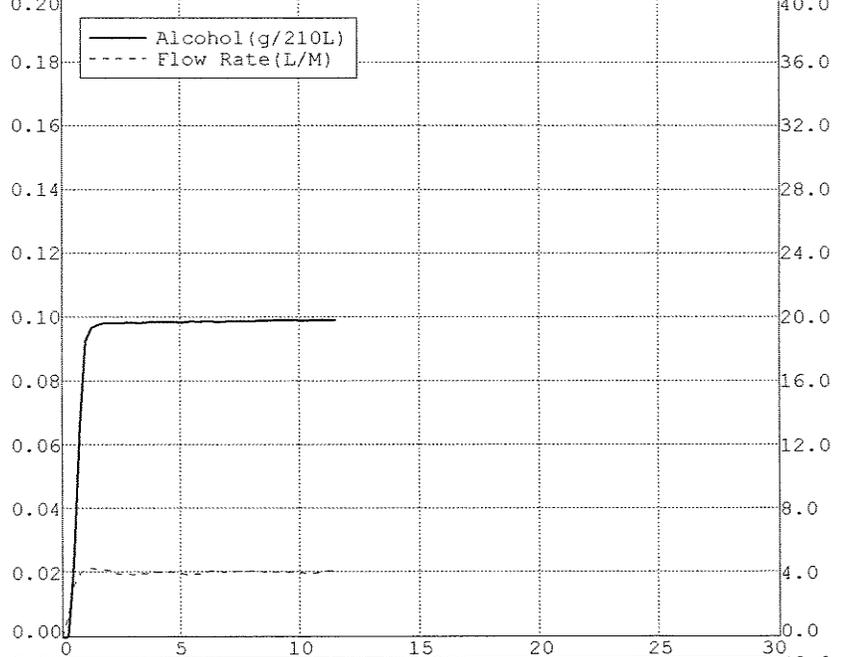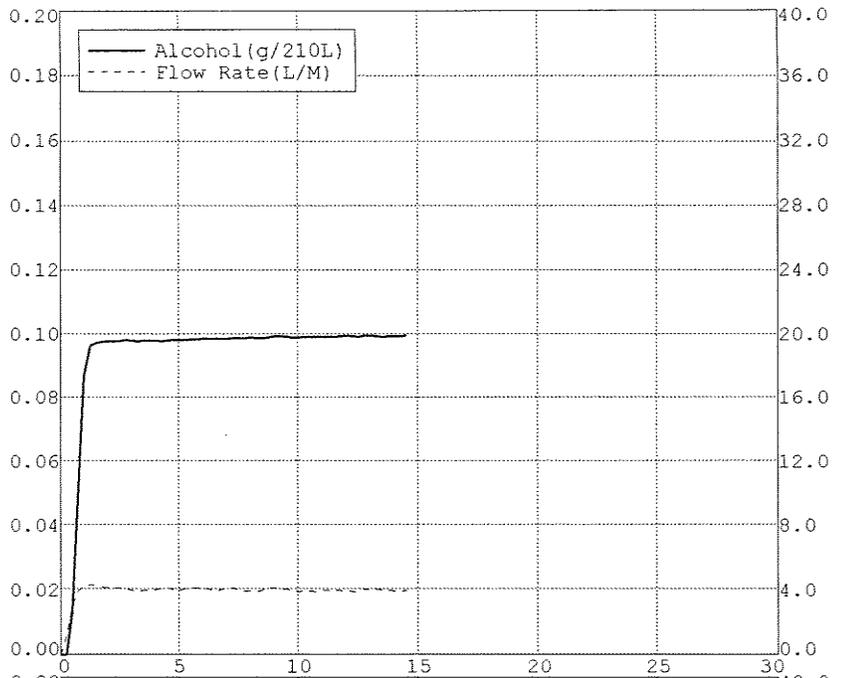

Charles B Geisler #211