

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 12/11/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:56
INTERNAL STANDARD	VERIFIED	00:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:56
BLANK TEST	0.00	00:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:58
BLANK TEST	0.00	00:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:59
BLANK TEST	0.00	01:00

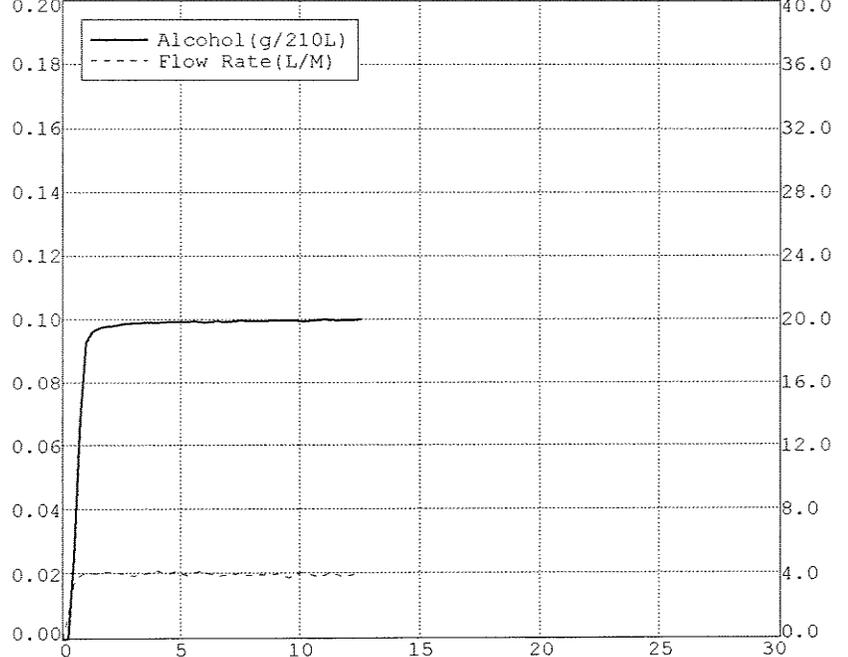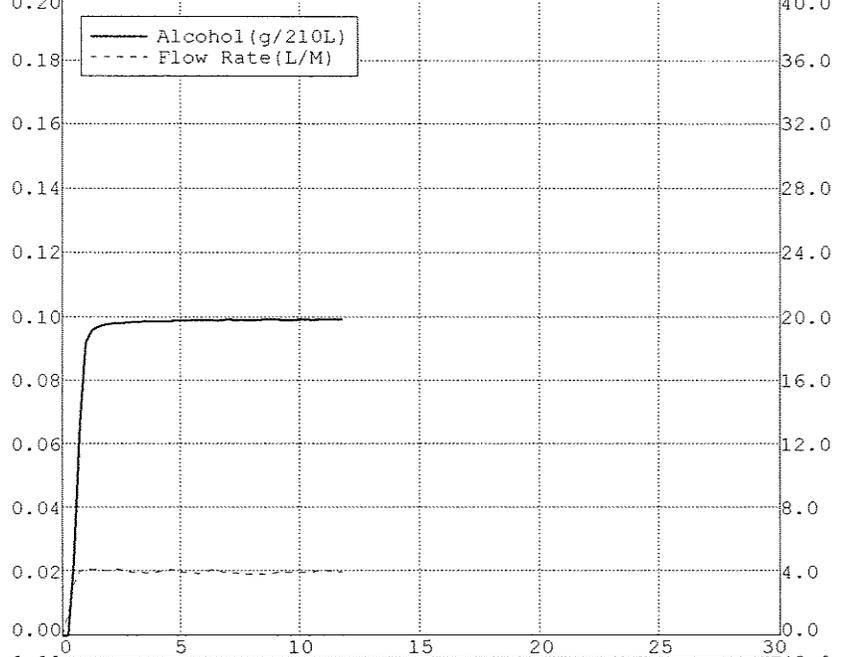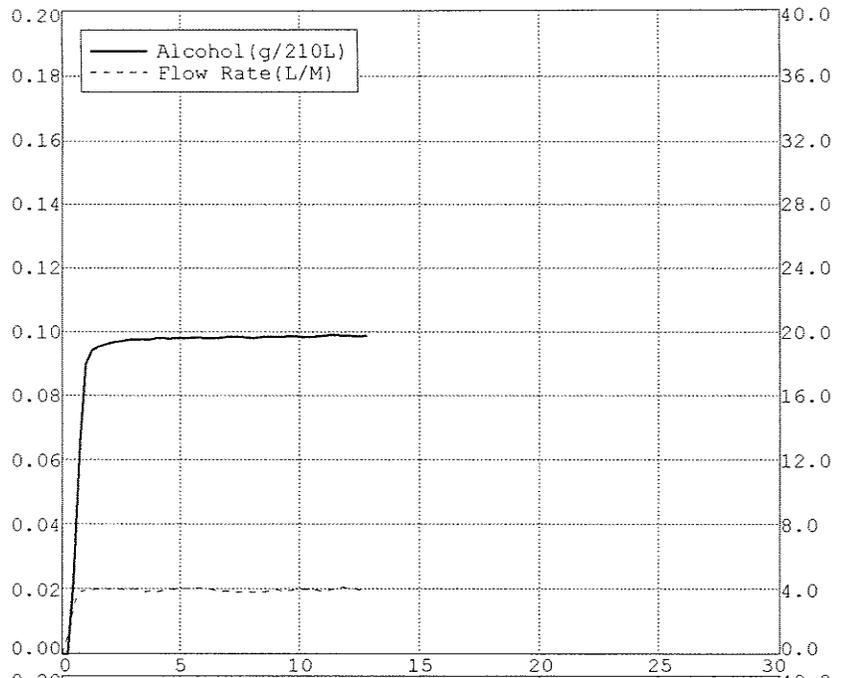

Handwritten signatures and initials:
C. B. Geisler
[Signature]
[Initials]

SUPERVISOR TEST

WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 12/11/2018

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 18310

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:49
INTERNAL STANDARD	VERIFIED	00:49
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:49
BLANK TEST	0.00	00:50
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	00:50
BLANK TEST	0.00	00:51
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	00:52

Blank Error

